


LB129785

7470A

INSTRUMENT ID: CV1

Linear

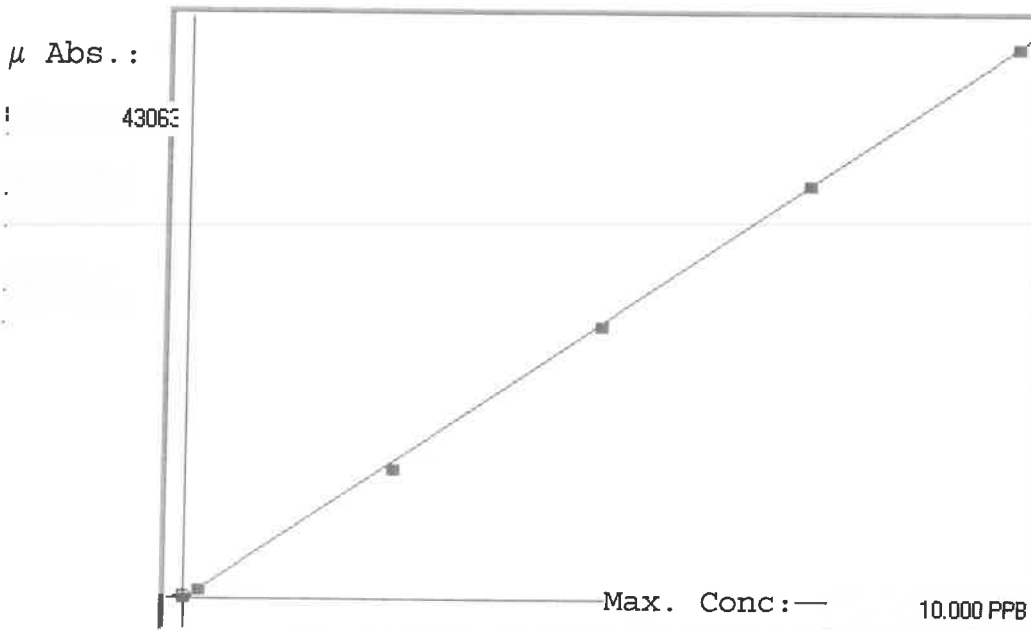

A= 0.0000e+000

B= 2.3184e-004

C= 2.6516e-002

Rho= 0.9998777

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.072	0.072	198	0.000	198	0				
0.2	0.200	0.216	0.016	817	0.0 %	817					
2.5	2.500	2.386	-0.114	10179	0.0 %	10179					
5.0	5.000	4.982	-0.018	21373	0.0 %	21373					
7.5	7.500	7.534	0.034	32381	0.0 %	32381					
10.0	10.000	10.010	0.010	43063	0.0 %	43063					

000500

LB129785 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Mar 2024 08:50:17

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	5.0	198	-	0.0000	7470A	PPB	06 Mar 2024 08:57:39	S	Std
0.2 - 1	5.2	817	-	0.2000	7470A	PPB	06 Mar 2024 08:59:56	S	Std
2.5 - 1	5.5	10179	-	2.5000	7470A	PPB	06 Mar 2024 09:02:13	S	Std
5.0 - 1	5.5	21373	-	5.0000	7470A	PPB	06 Mar 2024 09:06:28	S	Std
7.5 - 1	5.5	32381	-	7.5000	7470A	PPB	06 Mar 2024 09:09:19	S	Std
10.0 - 1	5.5	43063	-	10.0000	7470A	PPB	06 Mar 2024 09:11:34	S	Std
ICV35 - 1	ICV35	16553	3.8641	-	7470A	PPB	06 Mar 2024 09:15:58	U	SMPL
ICB35 - 1	ICB35	-109	0.0012	-	7470A	PPB	06 Mar 2024 09:18:55	U	SMPL
CCV30 - 1	CCV30	21548	5.0221	-	7470A	PPB	06 Mar 2024 09:22:58	U	SMPL
CCB30 - 1	CCB30	-109	0.0012	-	7470A	PPB	06 Mar 2024 09:25:51	U	SMPL
CRA - 1	CRA	718	0.1930	-	7470A	PPB	06 Mar 2024 09:28:05	U	SMPL
HighStd - 1	HighStd	43324	10.0706	-	7470A	PPB	06 Mar 2024 09:30:21	U	SMPL
ChkStd - 1	ChkStd	30810	7.1694	-	7470A	PPB	06 Mar 2024 09:32:38	U	SMPL
PB159454BL - 1	PBW	83	0.0458	-	7470A	PPB	06 Mar 2024 09:34:59	U	SMPL
PB159454BS - 1	LCSW	14608	3.4132	-	7470A	PPB	06 Mar 2024 09:36:52	U	SMPL
P1662-02 - 1	ETGI-352	-174	-0.0138	-	7470A	PPB	06 Mar 2024 09:39:08	U	SMPL
P1662-04 - 1	RBR-2520556	-42	0.0168	-	7470A	PPB	06 Mar 2024 09:41:27	U	SMPL
P1669-04 - 1	TP-14	11	0.0291	-	7470A	PPB	06 Mar 2024 09:43:43	U	SMPL
P1669-08 - 1	TP-11	18	0.0307	-	7470A	PPB	06 Mar 2024 09:48:04	U	SMPL
P1669-12 - 1	TP-6	41	0.0360	-	7470A	PPB	06 Mar 2024 09:50:19	U	SMPL
CCV31 - 1	CCV31	21313	4.9676	-	7470A	PPB	06 Mar 2024 09:52:34	U	SMPL
CCB31 - 1	CCB31	-258	-0.0333	-	7470A	PPB	06 Mar 2024 09:54:50	U	SMPL
P1669-12DUP - 1	TP-6DUP	36	0.0349	-	7470A	PPB	06 Mar 2024 09:59:06	U	SMPL
P1669-12MS - 1	TP-6MS	13815	3.2293	-	7470A	PPB	06 Mar 2024 10:01:21	U	SMPL
P1669-12MSD - 1	TP-6MSD	14529	3.3949	-	7470A	PPB	06 Mar 2024 10:03:36	U	SMPL
PB159401TB - 1	PB159401TB	79	0.0448	-	7470A	PPB	06 Mar 2024 10:05:55	U	SMPL
P1669-12LX5 - 1		-54	0.0140	-	7470A	PPB	06 Mar 2024 10:07:49	U	SMPL
P1669-12A - 1		16131	3.7663	-	7470A	PPB	06 Mar 2024 10:10:05	U	SMPL
CCV32 - 1	CCV32	21189	4.9389	-	7470A	PPB	06 Mar 2024 10:12:54	U	SMPL
CCB32 - 1	CCB32	-288	-0.0403	-	7470A	PPB	06 Mar 2024 10:15:11	U	SMPL