


LB129790

7471B

INSTRUMENT ID: CV2

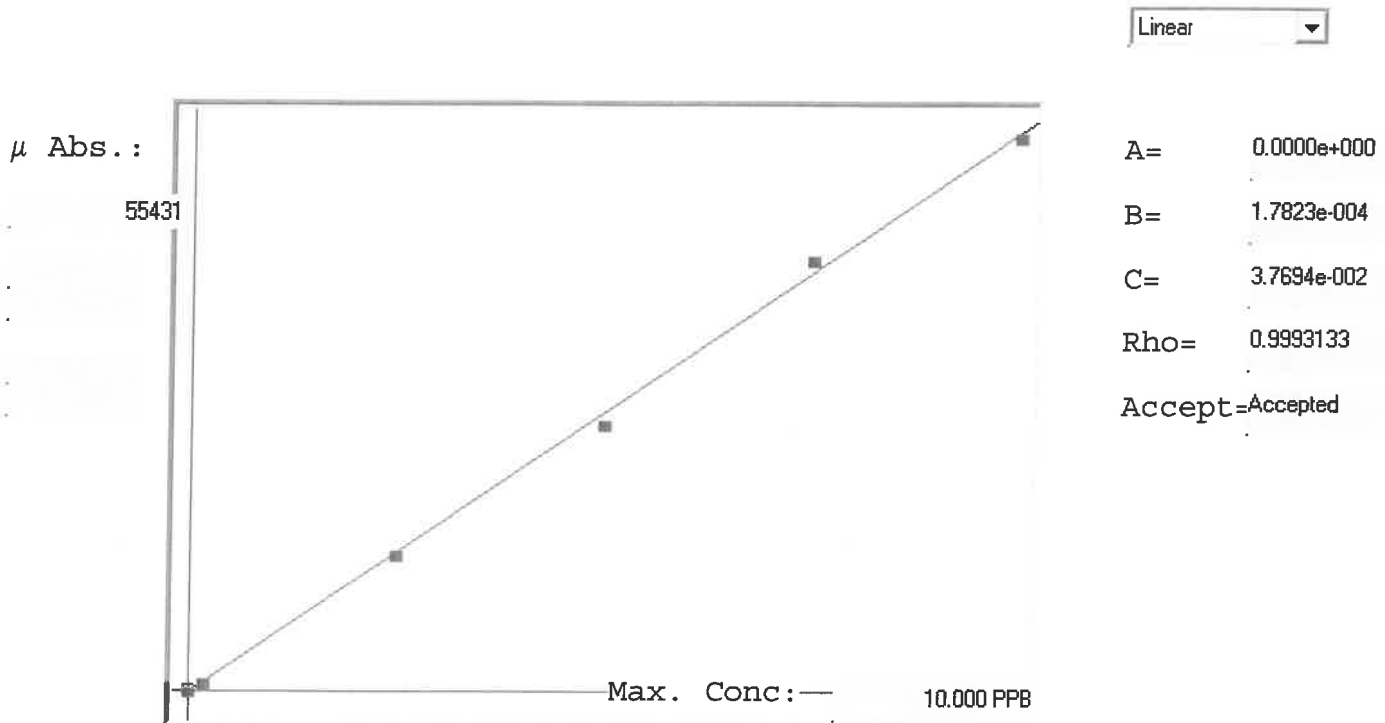

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	V/O
0.0	0.000	0.059	0.059	118	0.000	118					1
0.2	0.200	0.206	0.006	945	0.0 %	945					3
2.5	2.500	2.489	-0.011	13755	0.0 %	13755					0
5.0	5.000	4.789	-0.211	26661	0.0 %	26661					-4
7.5	7.500	7.739	0.239	43213	0.0 %	43213					3
10.0	10.000	9.917	-0.083	55431	0.0 %	55431					1

LB129790 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 06 Mar 2024 11:53:07

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	118	-	0.0000	7471B	PPB	06 Mar 2024 12:15:50	S	Std
0.2 - 1	50.2	945	-	0.2000	7471B	PPB	06 Mar 2024 12:18:08	S	Std
2.5 - 1	52.5	13755	-	2.5000	7471B	PPB	06 Mar 2024 12:20:25	S	Std
5.0 - 1	55	26661	-	5.0000	7471B	PPB	06 Mar 2024 12:22:42	S	Std
7.5 - 1	57.5	43213	-	7.5000	7471B	PPB	06 Mar 2024 12:25:01	S	Std
10.0 - 1	59	55431	-	10.0000	7471B	PPB	06 Mar 2024 12:27:22	S	Std
ICV36 - 1	ICV36	22343	4.0198	-	7471B	PPB	06 Mar 2024 12:30:26	U	SMPL
ICB36 - 1	ICB36	-203	0.0019	-	7471B	PPB	06 Mar 2024 12:32:41	U	SMPL
CCV33 - 1	CCV33	26966	4.8438	-	7471B	PPB	06 Mar 2024 12:35:01	U	SMPL
CCB33 - 1	CCB33	-187	0.0044	-	7471B	PPB	06 Mar 2024 12:37:16	U	SMPL
CRA - 1	CRA	890	0.1963	-	7471B	PPB	06 Mar 2024 12:39:38	U	SMPL
HighStd - 1	HighStd	55438	9.9183	-	7471B	PPB	06 Mar 2024 12:41:53	U	SMPL
ChkStd - 1	ChkStd	39528	7.0827	-	7471B	PPB	06 Mar 2024 12:44:09	U	SMPL
PB159476BL - 1	PBS	-275	-0.0113	-	7471B	PPB	06 Mar 2024 12:46:35	U	SMPL
P1326-01 - 1	1	5203	0.9650	-	7471B	PPB	06 Mar 2024 12:53:07	U	SMPL
P1662-01 - 1	ETGI-352	579	0.1409	-	7471B	PPB	06 Mar 2024 12:55:26	U	SMPL
P1662-03 - 1	RBR-2520556	1480	0.3015	-	7471B	PPB	06 Mar 2024 12:57:46	U	SMPL
P1666-01 - 1	OR-02-030124	2830	0.5421	-	7471B	PPB	06 Mar 2024 13:00:03	U	SMPL
P1666-01DUP - 1	OR-02-030124DUP	3207	0.6093	-	7471B	PPB	06 Mar 2024 13:02:18	U	SMPL
CCV34 - 1	CCV34	26807	4.8155	-	7471B	PPB	06 Mar 2024 13:04:36	U	SMPL
CCB34 - 1	CCB34	-156	0.0099	-	7471B	PPB	06 Mar 2024 13:06:53	U	SMPL
P1666-01MS - 1	OR-02-030124MS	20298	3.6554	-	7471B	PPB	06 Mar 2024 13:09:14	U	SMPL
P1666-01MSD - 1	OR-02-030124MSD	20900	3.7627	-	7471B	PPB	06 Mar 2024 13:11:29	U	SMPL
P1669-01 - 1	TP-14	5612	1.0379	-	7471B	PPB	06 Mar 2024 13:13:49	U	SMPL
P1669-05 - 1	TP-11	416	0.1118	-	7471B	PPB	06 Mar 2024 13:16:09	U	SMPL
P1669-09 - 1	TP-6	2774	0.5321	-	7471B	PPB	06 Mar 2024 13:18:27	U	SMPL
P1672-01 - 1	TP-1	7212	1.3231	-	7471B	PPB	06 Mar 2024 13:20:44	U	SMPL
P1672-05 - 1	TP-3	353	0.1006	-	7471B	PPB	06 Mar 2024 13:23:01	U	SMPL
P1672-09 - 1	TP-5	-14	0.0352	-	7471B	PPB	06 Mar 2024 13:25:21	U	SMPL
P1672-13 - 1	TP-13	517	0.1298	-	7471B	PPB	06 Mar 2024 13:27:37	U	SMPL
P1674-01 - 1	1A	4883	0.9080	-	7471B	PPB	06 Mar 2024 13:29:53	U	SMPL
CCV35 - 1	CCV35	27030	4.8552	-	7471B	PPB	06 Mar 2024 13:32:08	U	SMPL
CCB35 - 1	CCB35	-153	0.0104	-	7471B	PPB	06 Mar 2024 13:34:26	U	SMPL
P1674-03 - 1	2B	4086	0.7659	-	7471B	PPB	06 Mar 2024 13:36:47	U	SMPL
P1682-01 - 1	HR-04-03052024	2134	0.4180	-	7471B	PPB	06 Mar 2024 13:39:03	U	SMPL
P1683-01 - 1	1132	92	0.0541	-	7471B	PPB	06 Mar 2024 13:41:21	U	SMPL
P1684-01 - 1	SU-03-030524	2136	0.4184	-	7471B	PPB	06 Mar 2024 13:43:37	U	SMPL
P1685-01 - 1	72-12002	4639	0.8645	-	7471B	PPB	06 Mar 2024 13:45:53	U	SMPL
PB159476BS - 1	LCSS	21978	3.9548	-	7471B	PPB	06 Mar 2024 13:48:10	U	SMPL
P1666-01LX5 - 1		467	0.1209	-	7471B	PPB	06 Mar 2024 13:50:28	U	SMPL
P1666-01A - 1		22471	4.0427	-	7471B	PPB	06 Mar 2024 14:00:33	U	SMPL
P1672-09 - 1	TP-5	2894	0.5535	-	7471B	PPB	06 Mar 2024 14:25:16	U	SMPL
CCV36 - 1	CCV36	27651	4.9659	-	7471B	PPB	06 Mar 2024 14:27:57	U	SMPL
CCB36 - 1	CCB36	-140	0.0127	-	7471B	PPB	06 Mar 2024 14:30:12	U	SMPL