


LB129205

7470A

INSTRUMENT ID: CV2

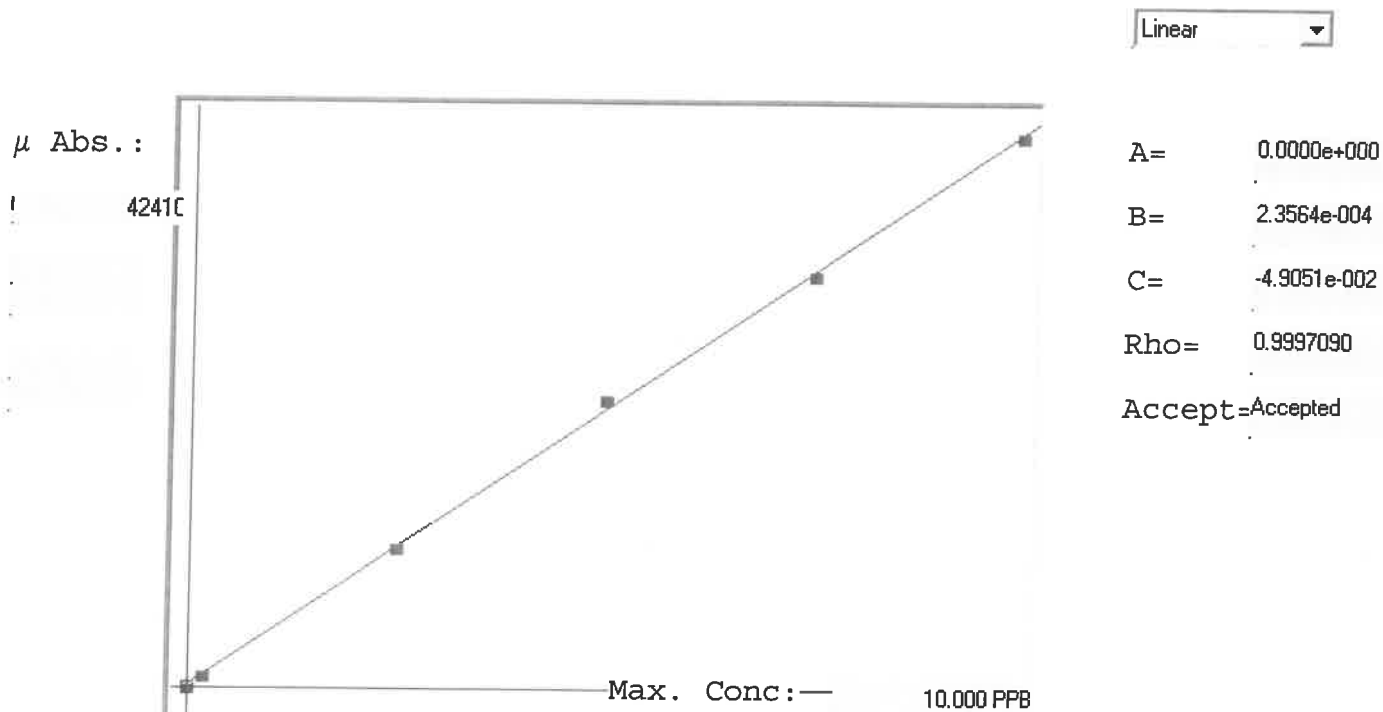

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.040	-0.040	38	0.000	38	0			
0.2	0.200	0.172	-0.028	940	0.0 %	940				
2.5	2.500	2.484	-0.016	10749	0.0 %	10749				
5.0	5.000	5.196	0.196	22261	0.0 %	22261				
7.5	7.500	7.443	-0.057	31796	0.0 %	31796				
10.0	10.000	9.944	-0.056	42410	0.0 %	42410				

LB129805 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 07 Mar 2024 12:17:02

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	38	-	0.0000	7470A	PPB	07 Mar 2024 13:17:22	S	Std
0.2 - 1	50.2	940	-	0.2000	7470A	PPB	07 Mar 2024 13:19:47	S	Std
2.5 - 1	52.5	10749	-	2.5000	7470A	PPB	07 Mar 2024 13:22:04	S	Std
5.0 - 1	53	22261	-	5.0000	7470A	PPB	07 Mar 2024 13:24:22	S	Std
7.5 - 1	53.5	31796	-	7.5000	7470A	PPB	07 Mar 2024 13:26:40	S	Std
10.0 - 1	53.8	42410	-	10.0000	7470A	PPB	07 Mar 2024 13:28:58	S	Std
ICV39 - 1	ICV39	17511	4.0772	-	7470A	PPB	07 Mar 2024 13:32:55	U	SMPL
ICB39 - 1	ICB39	-191	-0.0941	-	7470A	PPB	07 Mar 2024 13:35:09	U	SMPL
CCV41 - 1	CCV41	22224	5.1877	-	7470A	PPB	07 Mar 2024 13:37:27	U	SMPL
CCB41 - 1	CCB41	-207	-0.0978	-	7470A	PPB	07 Mar 2024 13:39:42	U	SMPL
CRA - 1	CRA	1100	0.2101	-	7470A	PPB	07 Mar 2024 13:41:59	U	SMPL
HighStd - 1	HighStd	42295	9.9171	-	7470A	PPB	07 Mar 2024 13:44:14	U	SMPL
ChkStd - 1	ChkStd	29020	6.7891	-	7470A	PPB	07 Mar 2024 13:46:30	U	SMPL
PB159491BL - 1	PBW	-7	-0.0507	-	7470A	PPB	07 Mar 2024 13:51:23	U	SMPL
PB159491BS - 1	LCSW	17371	4.0442	-	7470A	PPB	07 Mar 2024 13:56:19	U	SMPL
P1672-04 - 1	TP-1	-175	-0.0903	-	7470A	PPB	07 Mar 2024 13:58:35	U	SMPL
P1672-08 - 1	TP-3	-17	-0.0531	-	7470A	PPB	07 Mar 2024 14:00:54	U	SMPL
P1672-12 - 1	TP-5	-4	-0.0500	-	7470A	PPB	07 Mar 2024 14:03:11	U	SMPL
P1672-16 - 1	TP-13	62	-0.0344	-	7470A	PPB	07 Mar 2024 14:05:28	U	SMPL
P1673-01 - 1	RT-2321	32	-0.0415	-	7470A	PPB	07 Mar 2024 14:07:43	U	SMPL
CCV42 - 1	CCV42	21633	5.0484	-	7470A	PPB	07 Mar 2024 14:09:58	U	SMPL
CCB42 - 1	CCB42	-3	-0.0498	-	7470A	PPB	07 Mar 2024 14:15:14	U	SMPL
P1673-01DUP - 1	RT-2321DUP	114	-0.0222	-	7470A	PPB	07 Mar 2024 14:17:29	U	SMPL
P1673-01MS - 1	RT-2321MS	17640	4.1076	-	7470A	PPB	07 Mar 2024 14:19:45	U	SMPL
P1673-01MSD - 1	RT-2321MSD	17557	4.0880	-	7470A	PPB	07 Mar 2024 14:22:00	U	SMPL
P1673-01LX5 - 1		-151	-0.0846	-	7470A	PPB	07 Mar 2024 14:24:18	U	SMPL
P1673-01A - 1		17786	4.1420	-	7470A	PPB	07 Mar 2024 14:26:36	U	SMPL
PB159429TB - 1	PB159429TB	-202	-0.0966	-	7470A	PPB	07 Mar 2024 14:28:52	U	SMPL
CCV43 - 1	CCV43	22192	5.1802	-	7470A	PPB	07 Mar 2024 14:31:11	U	SMPL
CCV43 - 1	CCV43	-15	-0.0526	-	7470A	PPB	07 Mar 2024 14:36:01	U	SMPL