


LB129820

7471B

INSTRUMENT ID: CV1

Linear

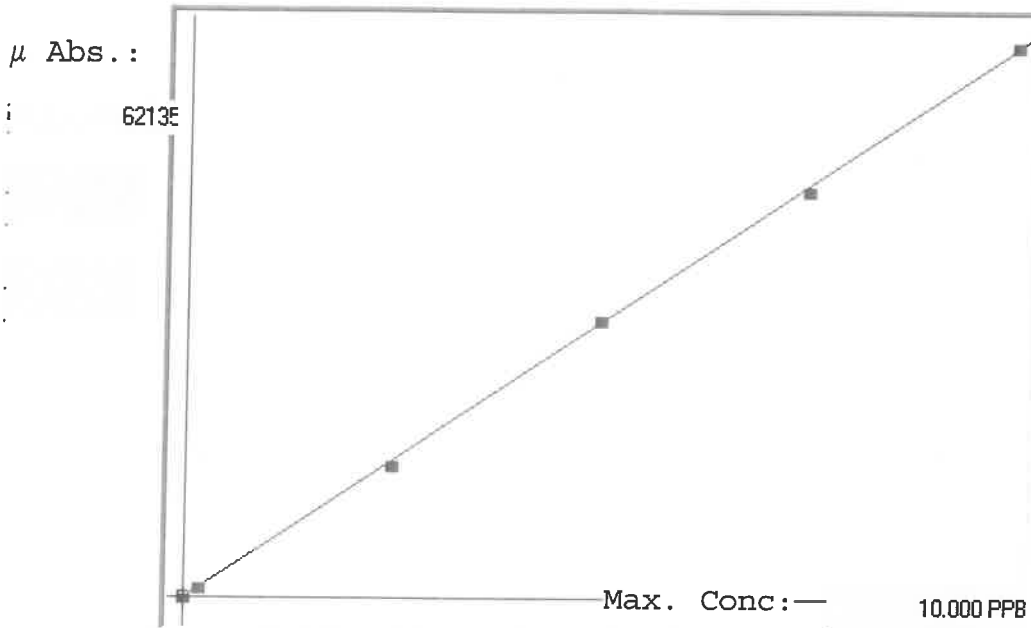

A= 0.0000e+000

B= 1.6135e-004

C= 1.4229e-002

Rho= 0.9999051

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/1)
0.0	0.000	0.019	0.019	27	0.000	27					
0.2	0.200	0.219	0.019	1270	0.0 %	1270					9
2.5	2.500	2.437	-0.063	15016	0.0 %	15016					-3
5.0	5.000	5.060	0.060	31273	0.0 %	31273					1
7.5	7.500	7.425	-0.075	45929	0.0 %	45929					-1
10.0	10.000	10.040	0.040	62135	0.0 %	62135					0

LB129820 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 08 Mar 2024 10:59:48

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	27	-	0.0000	7471B	PPB	08 Mar 2024 11:07:09	S	Std
0.2 - 1	50.2	1270	-	0.2000	7471B	PPB	08 Mar 2024 11:09:26	S	Std
2.5 - 1	52.5	15016	-	2.5000	7471B	PPB	08 Mar 2024 11:11:44	S	Std
5.0 - 1	55	31273	-	5.0000	7471B	PPB	08 Mar 2024 11:14:00	S	Std
7.5 - 1	57.5	45929	-	7.5000	7471B	PPB	08 Mar 2024 11:16:20	S	Std
10.0 - 1	510	62135	-	10.0000	7471B	PPB	08 Mar 2024 11:18:41	S	Std
ICV40 - 1	ICV40	25558	4.1381	-	7471B	PPB	08 Mar 2024 11:21:41	U	SMPL
ICB40 - 1	ICB40	-441	-0.0569	-	7471B	PPB	08 Mar 2024 11:23:57	U	SMPL
CCV43 - 1	CCV43	31332	5.0697	-	7471B	PPB	08 Mar 2024 11:26:15	U	SMPL
CCB43 - 1	CCB43	-179	-0.0147	-	7471B	PPB	08 Mar 2024 11:29:06	U	SMPL
CRA - 1	CRA	1237	0.2138	-	7471B	PPB	08 Mar 2024 11:31:23	U	SMPL
HighStd - 1	HighStd	62034	10.0236	-	7471B	PPB	08 Mar 2024 11:33:37	U	SMPL
ChkStd - 1	ChkStd	43467	7.0278	-	7471B	PPB	08 Mar 2024 11:35:53	U	SMPL
PB159508BL - 1	PBS	-272	-0.0297	-	7471B	PPB	08 Mar 2024 11:38:21	U	SMPL
PB159508BS - 1	LCSS	27051	4.3790	-	7471B	PPB	08 Mar 2024 11:40:46	U	SMPL
P1688-01 - 1	COMP-1	18561	3.0091	-	7471B	PPB	08 Mar 2024 11:48:05	U	SMPL
P1688-01DUP - 1	COMP-1DUP	17752	2.8786	-	7471B	PPB	08 Mar 2024 11:50:23	U	SMPL
P1688-01MS - 1	COMP-1MS	46076	7.4487	-	7471B	PPB	08 Mar 2024 11:52:44	U	SMPL
P1688-01MSD - 1	COMP-1MSD	42611	6.8897	-	7471B	PPB	08 Mar 2024 11:55:05	U	SMPL
P1688-02 - 1	COMP-2	686	0.1249	-	7471B	PPB	08 Mar 2024 11:57:32	U	SMPL
CCV44 - 1	CCV44	31791	5.1438	-	7471B	PPB	08 Mar 2024 11:59:56	U	SMPL
CCB44 - 1	CCB44	-211	-0.0198	-	7471B	PPB	08 Mar 2024 12:02:11	U	SMPL
P1688-03 - 1	COMP-3	470	0.0901	-	7471B	PPB	08 Mar 2024 12:04:33	U	SMPL
P1688-04 - 1	COMP-4	18299	2.9668	-	7471B	PPB	08 Mar 2024 12:06:49	U	SMPL
P1688-05 - 1	COMP-5	18817	3.0504	-	7471B	PPB	08 Mar 2024 12:09:04	U	SMPL
P1701-01 - 1	RCA-1-COMP	3421	0.5662	-	7471B	PPB	08 Mar 2024 12:11:24	U	SMPL
P1701-02 - 1	RCA-2-COMP	2665	0.4442	-	7471B	PPB	08 Mar 2024 12:13:43	U	SMPL
P1701-03 - 1	RCA-3-COMP	3213	0.5327	-	7471B	PPB	08 Mar 2024 12:16:00	U	SMPL
P1705-01 - 1	TP-1	6188	1.0127	-	7471B	PPB	08 Mar 2024 12:18:18	U	SMPL
P1705-03 - 1	TP-2	5028	0.8255	-	7471B	PPB	08 Mar 2024 12:20:36	U	SMPL
P1705-05 - 1	TP-2B	2466	0.4121	-	7471B	PPB	08 Mar 2024 12:22:55	U	SMPL
CCV45 - 1	CCV45	31577	5.1093	-	7471B	PPB	08 Mar 2024 12:25:13	U	SMPL
CCB45 - 1	CCB45	-47	0.0066	-	7471B	PPB	08 Mar 2024 12:28:08	U	SMPL
P1688-01LX5 - 1		3330	0.5515	-	7471B	PPB	08 Mar 2024 12:30:23	U	SMPL
P1688-01A - 1		44589	7.2088	-	7471B	PPB	08 Mar 2024 12:32:38	U	SMPL
CCV46 - 1	CCV46	31856	5.1543	-	7471B	PPB	08 Mar 2024 12:34:56	U	SMPL
CCB46 - 1	CCB46	-225	-0.0221	-	7471B	PPB	08 Mar 2024 12:37:21	U	SMPL