


LB 129822

SFAM01.1

INSTRUMENT ID: CV 1

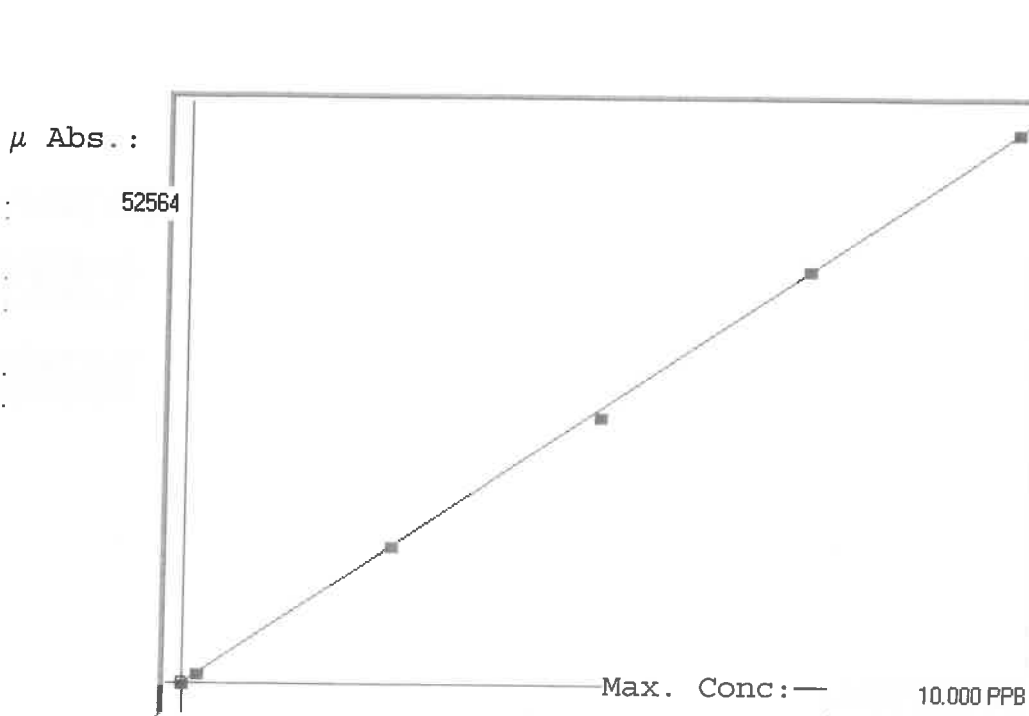

Linear

A= 0.0000e+000

B= 1.9053e-004 slope

C= 7.1118e-003 y-intercept

Rho= 0.9998529

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	C/D
0.00	0.000	0.031	0.031	127	0.000	127					0/1, D
0.05	0.050					442	0				5
0.20	0.200	0.210	0.010	1063	0.0 %	1063					1
2.50	2.500	2.524	0.024	13211	0.0 %	13211					-3
5.00	5.000	4.861	-0.139	25477	0.0 %	25477					1
7.50	7.500	7.551	0.051	39596	0.0 %	39596					0
10.0	10.000	10.022	0.022	52564	0.0 %	52564					

LB129822

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	127	-		0 SFAM01.1	PPB	3/8/2024 13:28	Std
	0.2 S01	1063	-		0.2 SFAM01.1	PPB	3/8/2024 13:30	Std
	2.5 S02	13211	-		2.5 SFAM01.1	PPB	3/8/2024 13:32	Std
	5 S03	25477	-		5 SFAM01.1	PPB	3/8/2024 13:35	Std
	7.5 S04	39596	-		7.5 SFAM01.1	PPB	3/8/2024 13:37	Std
	10 S05	52564	-		10 SFAM01.1	PPB	3/8/2024 13:42	Std
ICV041	ICV041	20189	3.8537 -		SFAM01.1	PPB	3/8/2024 13:45	SMPL
ICB041	ICB041	-104	-0.0127 -		SFAM01.1	PPB	3/8/2024 13:47	SMPL
CCV047	CCV047	25924	4.9464 -		SFAM01.1	PPB	3/8/2024 13:49	SMPL
CCB047	CCB047	-129	-0.0175 -		SFAM01.1	PPB	3/8/2024 13:52	SMPL
PB159520BL	PBW520	3	0.0077 -		SFAM01.1	PPB	3/8/2024 13:54	SMPL
PB159422TB	LEB422	85	0.0233 -		SFAM01.1	PPB	3/8/2024 13:56	SMPL
PB159423TB	LEB423	91	0.0245 -		SFAM01.1	PPB	3/8/2024 13:58	SMPL
P1644-01	MDCNI2	52	0.017 -		SFAM01.1	PPB	3/8/2024 14:01	SMPL
P1644-02	MDCNI2D	66	0.0197 -		SFAM01.1	PPB	3/8/2024 14:03	SMPL
P1644-03	MDCNI2S	4822	0.9259 -		SFAM01.1	PPB	3/8/2024 14:08	SMPL
P1644-05	MDCNI3	19	0.0107 -		SFAM01.1	PPB	3/8/2024 14:10	SMPL
P1644-06	MDCNI3D	58	0.0182 -		SFAM01.1	PPB	3/8/2024 14:12	SMPL
P1644-07	MDCNI3S	4671	0.8971 -		SFAM01.1	PPB	3/8/2024 14:17	SMPL
CCV048	CCV048	25306	4.8287 -		SFAM01.1	PPB	3/8/2024 14:19	SMPL
CCB048	CCB048	-130	-0.0177 -		SFAM01.1	PPB	3/8/2024 14:21	SMPL