

6129843

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

3/11/2024 13:36

Test: Phenolics-

Sample Id	nd Result	Dil. 1 +	Response	Errors
ICV1	0.999	0.0	0.107	
ICB1	0.005	0.0	0.013	
CCV1	0.995	0.0	0.106	
CCB1	-0.001	0.0	0.012	
PB159540BL	-0.003	0.0	0.012	
PB159540BS	0.991	0.0	0.106	
P1700-06	0.006	0.0	0.013	
P1700-04	0.006	0.0	0.013	
P1700-04DUP	0.005	0.0	0.013	
P1700-04MS	0.973	0.0	0.104	
P1700-04MSD	0.975	0.0	0.104	
CCV2	1.001	0.0	0.107	
CCB2	-0.000	0.0	0.013	

N 13
Mean 0.458
SD 0.5119
CV% 111.83

Aquakem v. 7.2AQ1

Results from time period:

Mon Mar 11 12:01:17 2024

Mon Mar 11 13:30:20 2024

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0028	mg/l	3/11/2024 12:18:54	
0.05PPM	A	Phenolics-	P	0.057	mg/l	3/11/2024 12:18:55	
0.1PPM	A	Phenolics-	P	0.1041	mg/l	3/11/2024 12:18:56	
0.25PPM	A	Phenolics-	P	0.2539	mg/l	3/11/2024 12:18:57	
0.50PPM	A	Phenolics-	P	0.4986	mg/l	3/11/2024 12:18:58	
1.0PPM	A	Phenolics-	P	0.9794	mg/l	3/11/2024 12:18:59	
2.0PPM	A	Phenolics-	P	2.0098	mg/l	3/11/2024 12:19:00	
ICV1	S	Phenolics-	P	0.9986	mg/l	3/11/2024 12:49:01	
ICB1	S	Phenolics-	P	0.0054	mg/l	3/11/2024 12:49:04	
CCV1	S	Phenolics-	P	0.9947	mg/l	3/11/2024 12:49:06	
CCB1	S	Phenolics-	P	-0.0013	mg/l	3/11/2024 12:49:08	
PB159540BL	S	Phenolics-	P	-0.0033	mg/l	3/11/2024 12:49:09	
PB159540BS	S	Phenolics-	P	0.9911	mg/l	3/11/2024 12:49:11	
P1700-06	S	Phenolics-	P	0.0059	mg/l	3/11/2024 12:59:11	
P1700-04	S	Phenolics-	P	0.0061	mg/l	3/11/2024 13:26:21	
P1700-04DUP	S	Phenolics-	P	0.0049	mg/l	3/11/2024 13:26:24	
P1700-04MS	S	Phenolics-	P	0.9731	mg/l	3/11/2024 13:26:25	
P1700-04MSD	S	Phenolics-	P	0.9747	mg/l	3/11/2024 13:26:27	
CCV2	S	Phenolics-	P	1.0011	mg/l	3/11/2024 13:26:29	
CCB2	S	Phenolics-	P	-0.0002	mg/l	3/11/2024 13:26:31	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

3/11/2024 12:19


Test Phenolics-

Accepted 3/11/2024 12:19

Factor 10.61
Bias 0.013

Coeff. of det. 0.999807

Errors

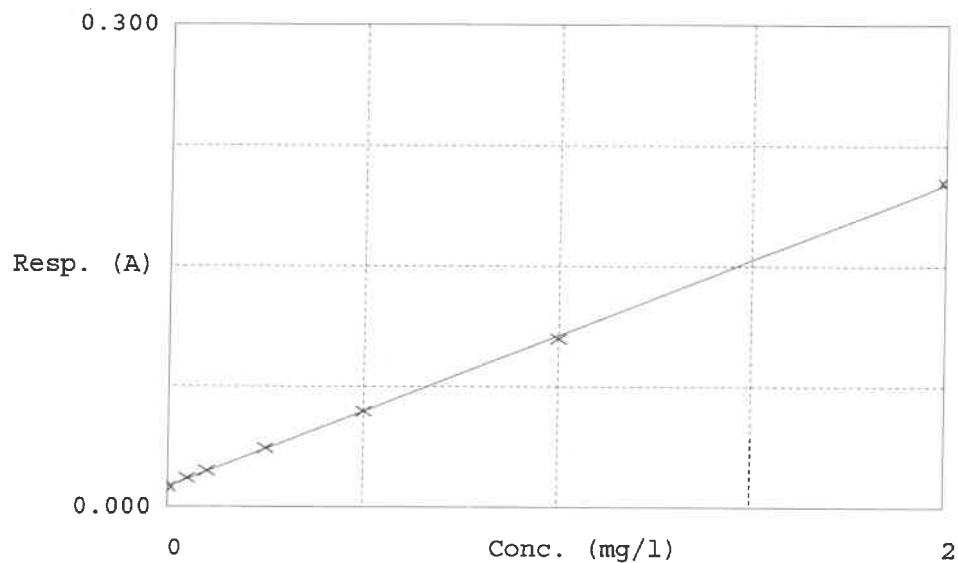

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.012	-0.0028	0.0000	
2	Phenol-2	0.018	0.0570	0.0500	14.0
3	Phenol-2	0.022	0.1041	0.1000	4.1
4	Phenol-2	0.037	0.2539	0.2500	1.6
5	Phenol-2	0.060	0.4986	0.5000	-0.3
6	Phenol-2	0.105	0.9794	1.0000	-2.1
7	Phenol-2	0.202	2.0098	2.0000	0.5

03/11/2024
RM