


LB129871

7470A

INSTRUMENT M: CV2

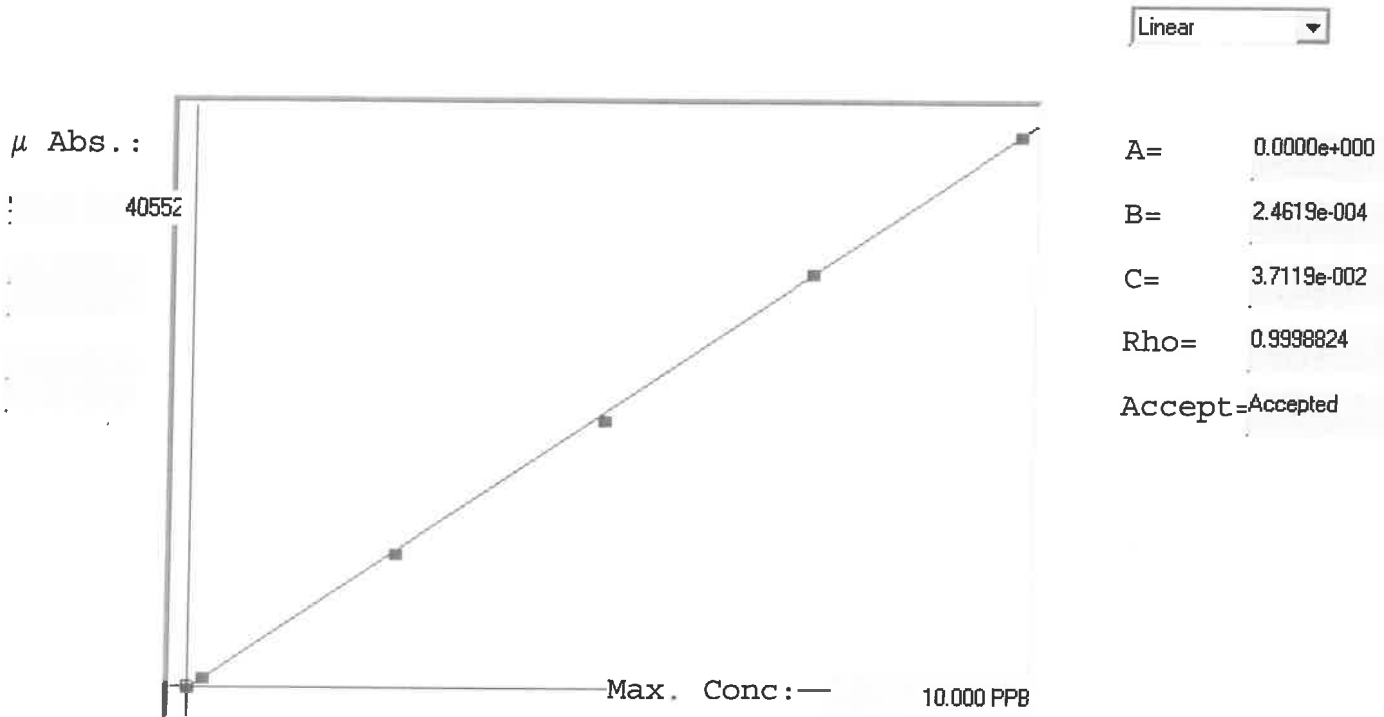

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	1/10
0.0	0.000	0.049	0.049	48	0.000	48	0				12
0.2	0.200	0.224	0.024	759	0.0 %	759					-2
2.5	2.500	2.459	-0.041	9836	0.0 %	9836					-2
5.0	5.000	4.894	-0.106	19729	0.0 %	19729					1
7.5	7.500	7.554	0.054	30533	0.0 %	30533					0
10.0	10.000	10.020	0.020	40552	0.0 %	40552					

LB129871 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Mar 2024 15:35:34

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	48	-	0.0000	7470A	PPB	13 Mar 2024 15:40:18	S	Std
0.2 - 1	50.2	759	-	0.2000	7470A	PPB	13 Mar 2024 15:43:09	S	Std
2.5 - 1	52.5	9836	-	2.5000	7470A	PPB	13 Mar 2024 15:45:26	S	Std
5.0 - 1	55	19729	-	5.0000	7470A	PPB	13 Mar 2024 15:47:43	S	Std
7.5 - 1	57.5	30533	-	7.5000	7470A	PPB	13 Mar 2024 15:50:01	S	Std
10.0 - 1	514	40552	-	10.0000	7470A	PPB	13 Mar 2024 15:52:19	S	Std
ICV47 - 1	ICV47	15634	3.8860	-	7470A	PPB	13 Mar 2024 15:55:20	U	SMPL
ICB47 - 1	ICB47	-231	-0.0198	-	7470A	PPB	13 Mar 2024 15:57:35	U	SMPL
CCV63 - 1	CCV63	19790	4.9091	-	7470A	PPB	13 Mar 2024 15:59:53	U	SMPL
CCB63 - 1	CCB63	-115	0.0088	-	7470A	PPB	13 Mar 2024 16:02:46	U	SMPL
CRA - 1	CRA	740	0.2193	-	7470A	PPB	13 Mar 2024 16:05:00	U	SMPL
HighStd - 1	HighStd	37092	9.1686	-	7470A	PPB	13 Mar 2024 16:07:15	U	SMPL
ChkStd - 1	ChkStd	27429	6.7898	-	7470A	PPB	13 Mar 2024 16:09:30	U	SMPL
PB159561BL - 1	PBW	-361	-0.0518	-	7470A	PPB	13 Mar 2024 16:11:51	U	SMPL
PB159561BS - 1	LCSW	16646	4.1351	-	7470A	PPB	13 Mar 2024 16:14:10	U	SMPL
P1725-02 - 1	RT-3860	-208	-0.0141	-	7470A	PPB	13 Mar 2024 16:16:27	U	SMPL
P1725-02DUP - 1	RT-3860DUP	-18	0.0327	-	7470A	PPB	13 Mar 2024 16:18:45	U	SMPL
P1725-02MS - 1	RT-3860MS	15738	3.9116	-	7470A	PPB	13 Mar 2024 16:21:02	U	SMPL
P1725-02MSD - 1	RT-3860MSD	16454	4.0879	-	7470A	PPB	13 Mar 2024 16:23:19	U	SMPL
PB159581BL - 1	PBW	-228	-0.0190	-	7470A	PPB	13 Mar 2024 16:25:37	U	SMPL
CCV64 - 1	CCV64	20073	4.9788	-	7470A	PPB	13 Mar 2024 16:27:54	U	SMPL
CCB64 - 1	CCB64	-232	-0.0200	-	7470A	PPB	13 Mar 2024 16:30:09	U	SMPL
PB159581BS - 1	LCSW	15969	3.9685	-	7470A	PPB	13 Mar 2024 16:32:28	U	SMPL
P1733-04 - 1	WC-1	-187	-0.0089	-	7470A	PPB	13 Mar 2024 16:34:43	U	SMPL
P1733-08 - 1	WC-2	-30	0.0297	-	7470A	PPB	13 Mar 2024 16:37:01	U	SMPL
P1733-12 - 1	WC-3	-1	0.0369	-	7470A	PPB	13 Mar 2024 16:40:51	U	SMPL
P1733-12DUP - 1	WC-3DUP	4	0.0381	-	7470A	PPB	13 Mar 2024 16:43:07	U	SMPL
P1733-12MS - 1	WC-3MS	16442	4.0849	-	7470A	PPB	13 Mar 2024 16:45:24	U	SMPL
P1733-12MSD - 1	WC-3MSD	15124	3.7604	-	7470A	PPB	13 Mar 2024 16:47:40	U	SMPL
PB159530TB - 1	PB159530TB	-208	-0.0141	-	7470A	PPB	13 Mar 2024 16:49:59	U	SMPL
PB159559TB - 1	PB159559TB	-3	0.0364	-	7470A	PPB	13 Mar 2024 16:52:18	U	SMPL
CCV65 - 1	CCV65	19500	4.8377	-	7470A	PPB	13 Mar 2024 16:54:34	U	SMPL
CCB65 - 1	CCB65	-229	-0.0193	-	7470A	PPB	13 Mar 2024 16:56:50	U	SMPL
P1725-02LX5 - 1		33	0.0452	-	7470A	PPB	13 Mar 2024 16:59:08	U	SMPL
P1725-02A - 1		15259	3.7937	-	7470A	PPB	13 Mar 2024 17:01:24	U	SMPL
P1733-12LX5 - 1		-109	0.0103	-	7470A	PPB	13 Mar 2024 17:03:40	U	SMPL
P1733-12A - 1		15111	3.7572	-	7470A	PPB	13 Mar 2024 17:05:58	U	SMPL
CCV66 - 1	CCV66	21154	5.2449	-	7470A	PPB	13 Mar 2024 17:08:14	U	SMPL
CCB66 - 1	CCB66	-288	-0.0338	-	7470A	PPB	13 Mar 2024 17:10:33	U	SMPL