


LB129889

7470A

INSTRUMENT ID: CV1

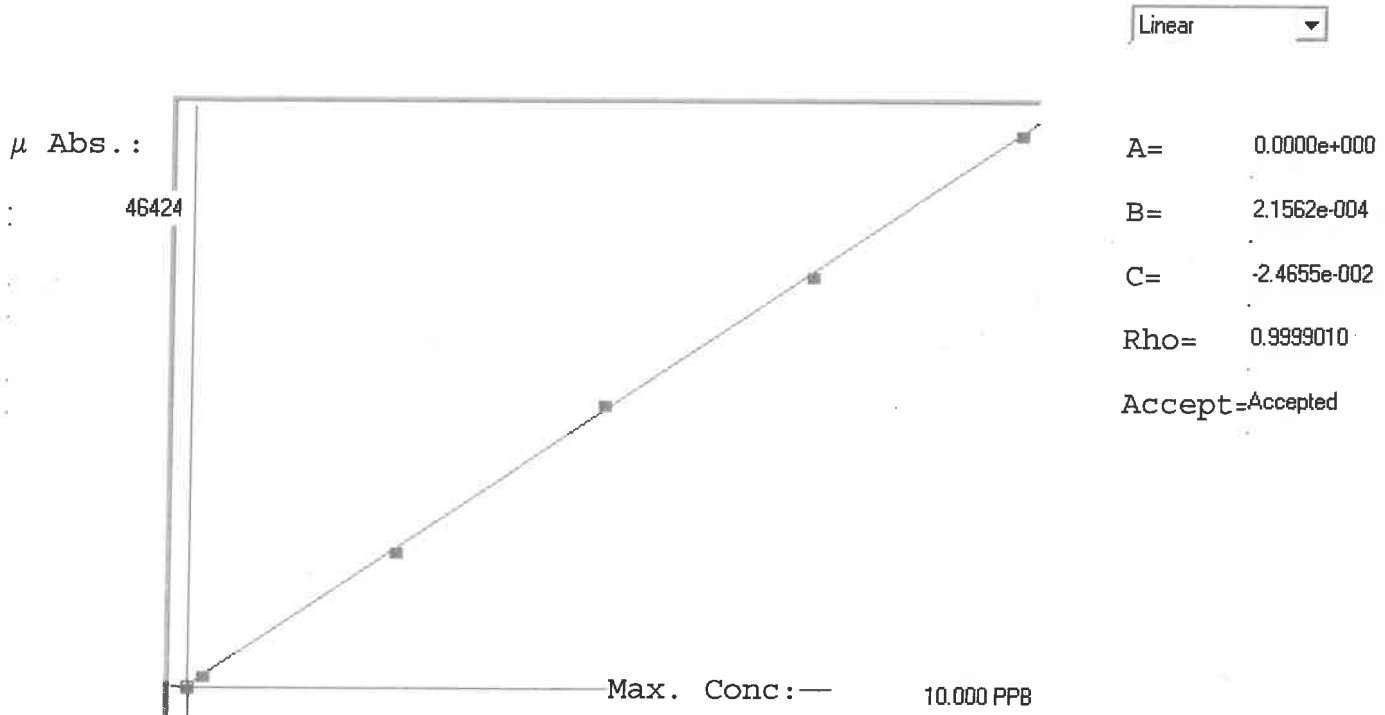

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/s)
0.0	0.000	-0.012	-0.012	61	0.000	61	0				—
0.2	0.200	0.196	-0.004	1023	0.0 %	1023					-2
2.5	2.500	2.463	-0.037	11538	0.0 %	11538					-1
5.0	5.000	5.112	0.112	23822	0.0 %	23822					2
7.5	7.500	7.456	-0.044	34693	0.0 %	34693					-1
10.0	10.000	9.985	-0.015	46424	0.0 %	46424					0

LB129889 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 14 Mar 2024 15:36:22

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SO	61	-	0.0000	7470A	PPB	14 Mar 2024 15:45:40	S	Std
0.2 - 1	SO.2	1023	-	0.2000	7470A	PPB	14 Mar 2024 15:47:58	S	Std
2.5 - 1	SO.5	11538	-	2.5000	7470A	PPB	14 Mar 2024 15:50:15	S	Std
5.0 - 1	SS	23822	-	5.0000	7470A	PPB	14 Mar 2024 15:52:31	S	Std
7.5 - 1	SS	34693	-	7.5000	7470A	PPB	14 Mar 2024 15:54:48	S	Std
10.0 - 1	CV	46424	-	10.0000	7470A	PPB	14 Mar 2024 16:02:24	S	Std
ICV49 - 1	ICV49	17497	3.7480	-	7470A	PPB	14 Mar 2024 16:07:50	U	SMPL
ICB49 - 1	ICB49	-142	-0.0553	-	7470A	PPB	14 Mar 2024 16:10:05	U	SMPL
CCV69 - 1	CCV69	22816	4.8953	-	7470A	PPB	14 Mar 2024 16:12:23	U	SMPL
CCB69 - 1	CCB69	-116	-0.0497	-	7470A	PPB	14 Mar 2024 16:14:37	U	SMPL
CRA - 1	CRA	924	0.1746	-	7470A	PPB	14 Mar 2024 16:16:55	U	SMPL
HighStd - 1	HighStd	53065	11.4170	-	7470A	PPB	14 Mar 2024 16:19:10	U	SMPL
ChkStd - 1	ChkStd	33208	7.1355	-	7470A	PPB	14 Mar 2024 16:21:25	U	SMPL
PB159601BL - 1	PBW	-298	-0.0889	-	7470A	PPB	14 Mar 2024 16:23:47	U	SMPL
PB159601BS - 1	LCSW	17892	3.8331	-	7470A	PPB	14 Mar 2024 16:26:06	U	SMPL
P1187-07 - 1	LOD-MDL-WATER-01-QT1-2024	297	0.0394	-	7470A	PPB	14 Mar 2024 16:36:12	U	SMPL
P1187-08 - 1	LOQ-WATER-02-QT1-2024	1020	0.1953	-	7470A	PPB	14 Mar 2024 16:38:28	U	SMPL
P1734-06 - 1	COMP-2	71	-0.0093	-	7470A	PPB	14 Mar 2024 16:40:45	U	SMPL
P1734-06DUP - 1	COMP-2DUP	90	-0.0052	-	7470A	PPB	14 Mar 2024 16:43:02	U	SMPL
P1734-06MS - 1	COMP-2MS	18751	4.0183	-	7470A	PPB	14 Mar 2024 16:45:17	U	SMPL
CCV70 - 1	CCV70	24280	5.2105	-	7470A	PPB	14 Mar 2024 16:47:32	U	SMPL
CCB70 - 1	CCB70	-129	-0.0525	-	7470A	PPB	14 Mar 2024 16:49:50	U	SMPL
P1734-06MSD - 1	COMP-2MSD	22007	4.7204	-	7470A	PPB	14 Mar 2024 16:52:07	U	SMPL
P1734-06LX5 - 1		-110	-0.0484	-	7470A	PPB	14 Mar 2024 16:54:22	U	SMPL
P1734-06A - 1		19798	4.2441	-	7470A	PPB	14 Mar 2024 16:56:40	U	SMPL
CCV71 - 1	CCV71	23992	5.1484	-	7470A	PPB	14 Mar 2024 17:01:32	U	SMPL
CCB71 - 1	CCB71	-95	-0.0451	-	7470A	PPB	14 Mar 2024 17:03:49	U	SMPL