


LB129901

SFAM01.1

INSTRUMENT ID: CV1

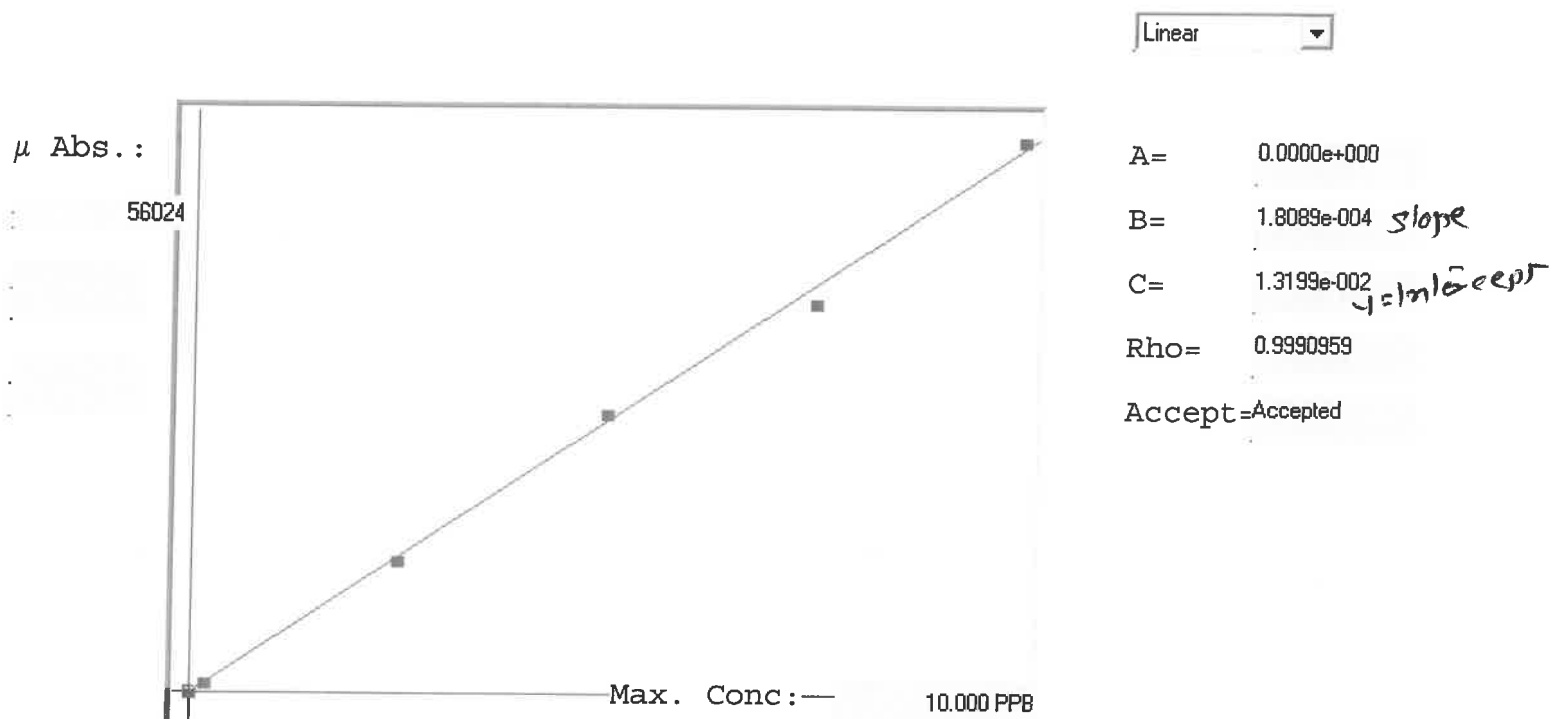

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/e))
0.00	0.000	0.023	0.023	56	0.000	56					1
0.05	0.050					442	0				10
0.20	0.200	0.219	0.019	1137	0.0 %	1137					-2
2.50	2.500	2.460	-0.040	13525	0.0 %	13525					3
5.00	5.000	5.162	0.162	28463	0.0 %	28463					-4
7.50	7.500	7.188	-0.312	39665	0.0 %	39665					1
10.0	10.000	10.148	0.148	56024	0.0 %	56024					

LB129901

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	56	-		0 SFAM01.1	PPB	3/15/2024 11:43	Std
	0.2 S01	1137	-		0.2 SFAM01.1	PPB	3/15/2024 11:45	Std
	2.5 S02	13525	-		2.5 SFAM01.1	PPB	3/15/2024 11:47	Std
	5 S03	28463	-		5 SFAM01.1	PPB	3/15/2024 11:50	Std
	7.5 S04	39665	-		7.5 SFAM01.1	PPB	3/15/2024 11:52	Std
	10 S05	56024	-		10 SFAM01.1	PPB	3/15/2024 11:54	Std
ICV051	ICV051	21904	3.9755 -		SFAM01.1	PPB	3/15/2024 12:00	SMPL
ICB051	ICB051	-178	-0.019 -		SFAM01.1	PPB	3/15/2024 12:02	SMPL
CCV075	CCV075	28627	5.1917 -		SFAM01.1	PPB	3/15/2024 12:04	SMPL
CCB075	CCB075	-206	-0.0241 -		SFAM01.1	PPB	3/15/2024 12:06	SMPL
PB159621BL	PBW621	0	0.0132 -		SFAM01.1	PPB	3/15/2024 12:09	SMPL
P1761-11	E0749	40	0.0204 -		SFAM01.1	PPB	3/15/2024 12:11	SMPL
CCV076	CCV076	28526	5.1734 -		SFAM01.1	PPB	3/15/2024 12:13	SMPL
CCB076	CCB076	-200	-0.023 -		SFAM01.1	PPB	3/15/2024 12:15	SMPL