


LB129911

7471B

INSTRUMENT ID: CV1

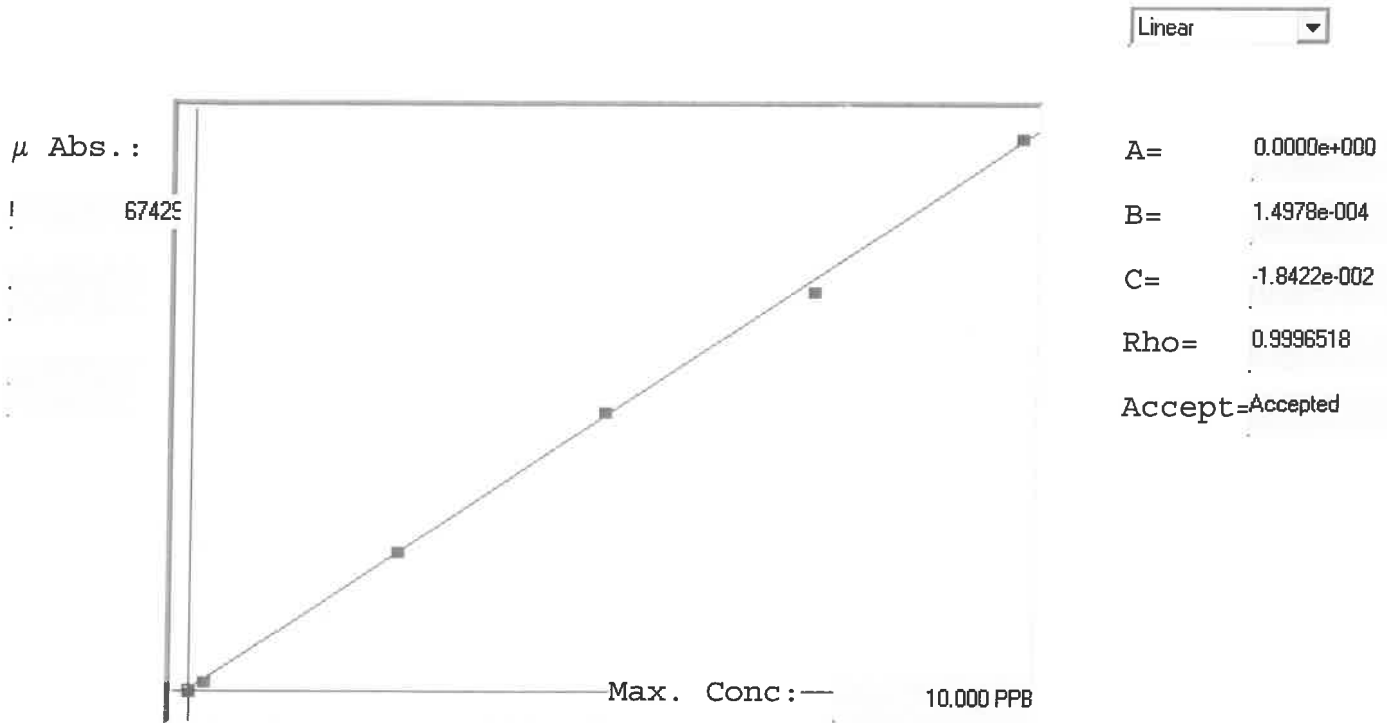

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	✓/1)
0.0	0.000	-0.016	-0.016	17	0.000	17					-
0.2	0.200	0.180	-0.020	1324	0.0 %	1324					-10
2.5	2.500	2.560	0.060	17217	0.0 %	17217					2
5.0	5.000	5.090	0.090	34103	0.0 %	34103					2
7.5	7.500	7.305	-0.195	48895	0.0 %	48895					-3
10.0	10.000	10.081	0.081	67429	0.0 %	67429					1

LB129911 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 15 Mar 2024 14:33:44

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	17	-	0.0000	7471B	PPB	15 Mar 2024 15:10:25	S	Std
0.2 - 1	50.2	1324	-	0.2000	7471B	PPB	15 Mar 2024 15:15:21	S	Std
2.5 - 1	52.5	17217	-	2.5000	7471B	PPB	15 Mar 2024 15:17:38	S	Std
5.0 - 1	35	34103	-	5.0000	7471B	PPB	15 Mar 2024 15:19:55	S	Std
7.5 - 1	37.5	48895	-	7.5000	7471B	PPB	15 Mar 2024 15:22:14	S	Std
10.0 - 1	310	67429	-	10.0000	7471B	PPB	15 Mar 2024 15:24:38	S	Std
ICV52 - 1	ICV52	25537	3.8065	-	7471B	PPB	15 Mar 2024 15:27:54	U	SMPL
ICB52 - 1	ICB52	513	0.0584	-	7471B	PPB	15 Mar 2024 15:30:09	U	SMPL
CCV77 - 1	CCV77	34524	5.1526	-	7471B	PPB	15 Mar 2024 15:32:30	U	SMPL
CCB77 - 1	CCB77	504	0.0571	-	7471B	PPB	15 Mar 2024 15:34:45	U	SMPL
CRA - 1	CRA	1299	0.1761	-	7471B	PPB	15 Mar 2024 15:37:09	U	SMPL
HighStd - 1	HighStd	67453	10.0847	-	7471B	PPB	15 Mar 2024 15:39:23	U	SMPL
ChkStd - 1	ChkStd	46083	6.8839	-	7471B	PPB	15 Mar 2024 15:41:39	U	SMPL
PB159629BL - 1	PBS	570	0.0670	-	7471B	PPB	15 Mar 2024 15:44:07	U	SMPL
PB159629BS - 1	LCSS	27110	4.0421	-	7471B	PPB	15 Mar 2024 15:46:32	U	SMPL
P1746-01 - 1	SB-01-0-2.0	19875	2.9585	-	7471B	PPB	15 Mar 2024 15:48:48	U	SMPL
P1746-02 - 1	SB-01-4.0-6.0	1800	0.2512	-	7471B	PPB	15 Mar 2024 15:51:11	U	SMPL
P1746-04 - 1	SB-01-7.0-9.5	37082	5.5357	-	7471B	PPB	15 Mar 2024 15:53:32	U	SMPL
P1746-06 - 1	SB-02-0-2.0	45749	6.8339	-	7471B	PPB	15 Mar 2024 15:55:50	U	SMPL
P1746-08 - 1	SB-03-0-2.0	32843	4.9008	-	7471B	PPB	15 Mar 2024 15:58:13	U	SMPL
CCV78 - 1	CCV78	34195	5.1033	-	7471B	PPB	15 Mar 2024 16:00:39	U	SMPL
CCB78 - 1	CCB78	312	0.0283	-	7471B	PPB	15 Mar 2024 16:03:02	U	SMPL
P1746-09 - 1	SB-03-2.0-3.0	32403	4.8349	-	7471B	PPB	15 Mar 2024 16:05:25	U	SMPL
P1746-11 - 1	SB-04-0-2.0	39725	5.9316	-	7471B	PPB	15 Mar 2024 16:07:40	U	SMPL
P1746-12 - 1	SB-04-2.0-4.0	28534	4.2554	-	7471B	PPB	15 Mar 2024 16:10:01	U	SMPL
P1746-13 - 1	SB-04-4.0-6.0	16415	2.4402	-	7471B	PPB	15 Mar 2024 16:12:25	U	SMPL
P1746-15 - 1	SB-05-0-2.0	29795	4.4443	-	7471B	PPB	15 Mar 2024 16:14:49	U	SMPL
P1746-16 - 1	SB-05-0-2.0-DUP	26273	3.9167	-	7471B	PPB	15 Mar 2024 16:17:09	U	SMPL
P1746-17 - 1	SB-05-2.0-4.5	32886	4.9072	-	7471B	PPB	15 Mar 2024 16:19:32	U	SMPL
P1746-19 - 1	SB-06-0-2.0	36678	5.4752	-	7471B	PPB	15 Mar 2024 16:21:53	U	SMPL
P1746-19DUP - 1	SB-06-0-2.0DUP	36466	5.4434	-	7471B	PPB	15 Mar 2024 16:24:17	U	SMPL
P1746-19MS - 1	SB-06-0-2.0MS	55913	8.3562	-	7471B	PPB	15 Mar 2024 16:29:33	U	SMPL
CCV79 - 1	CCV79	34104	5.0897	-	7471B	PPB	15 Mar 2024 16:31:50	U	SMPL
CCB79 - 1	CCB79	317	0.0291	-	7471B	PPB	15 Mar 2024 16:34:16	U	SMPL
P1746-19MSD - 1	SB-06-0-2.0MSD	57940	8.6598	-	7471B	PPB	15 Mar 2024 16:36:39	U	SMPL
P1764-10 - 1	COMP-1	2420	0.3440	-	7471B	PPB	15 Mar 2024 16:38:54	U	SMPL
P1764-11 - 1	COMP-2	4440	0.6466	-	7471B	PPB	15 Mar 2024 16:41:17	U	SMPL
P1767-01 - 1	NB-07-031424	7046	1.0369	-	7471B	PPB	15 Mar 2024 16:43:33	U	SMPL
P1772-01 - 1	1151	3547	0.5128	-	7471B	PPB	15 Mar 2024 16:45:51	U	SMPL
P1772-02 - 1	1276	3838	0.5564	-	7471B	PPB	15 Mar 2024 16:48:10	U	SMPL
P1774-01 - 1	TP3	3920	0.5687	-	7471B	PPB	15 Mar 2024 16:50:28	U	SMPL
P1774-02 - 1	TP9	3533	0.5108	-	7471B	PPB	15 Mar 2024 16:52:47	U	SMPL
P1746-19LX5 - 1		8511	1.2564	-	7471B	PPB	15 Mar 2024 16:55:06	U	SMPL
P1746-19A - 1		61334	9.1682	-	7471B	PPB	15 Mar 2024 16:57:23	U	SMPL
CCV80 - 1	CCV80	34146	5.0960	-	7471B	PPB	15 Mar 2024 16:59:41	U	SMPL
CCB80 - 1	CCB80	408	0.0427	-	7471B	PPB	15 Mar 2024 17:02:08	U	SMPL