

LB129944

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12 Instrument ID : Konelab

3/19/2024 14:09

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.932	0.0	0.100	
ICB1	0.002	0.0	0.007	
CCV1	0.973	0.0	0.104	
CCB1	-0.002	0.0	0.007	
PB159660BL	-0.002	0.0	0.007	
PB159660BS	0.936	0.0	0.100	
P1788-02	0.006	0.0	0.007	
P1788-02DUP	0.008	0.0	0.008	
P1788-01	-2.156	0.0	-0.209	
P1788-02MS	0.980	0.0	0.105	
P1788-02MSD	0.981	0.0	0.105	
CCV2	0.990	0.0	0.106	
CCB2	0.003	0.0	0.007	

N	13
Mean	0.281
SD	0.8765
CV%	312.11

Aquakem v. 7.2AQ1

Results from time period:

Tue Mar 19 12:56:03 2024

Tue Mar 19 14:00:44 2024

Sample Id	Sam/Ctr/cA	Test short n	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0017	mg/l	3/19/2024 12:56:03	
0.05PPM	A	Phenolics-	P	0.0591	mg/l	3/19/2024 12:56:04	
0.1PPM	A	Phenolics-	P	0.103	mg/l	3/19/2024 12:56:05	
0.25PPM	A	Phenolics-	P	0.25	mg/l	3/19/2024 12:56:06	
0.50PPM	A	Phenolics-	P	0.4969	mg/l	3/19/2024 12:56:07	
1.0PPM	A	Phenolics-	P	0.9847	mg/l	3/19/2024 12:56:08	
2.0PPM	A	Phenolics-	P	2.008	mg/l	3/19/2024 12:56:09	
ICV1	S	Phenolics-	P	0.9318	mg/l	3/19/2024 13:27:49	
ICB1	S	Phenolics-	P	0.0015	mg/l	3/19/2024 13:27:50	
CCV1	S	Phenolics-	P	0.9731	mg/l	3/19/2024 13:27:52	
CCB1	S	Phenolics-	P	-0.0019	mg/l	3/19/2024 13:27:55	
PB159660BL	S	Phenolics-	P	-0.0017	mg/l	3/19/2024 13:27:56	
PB159660BS	S	Phenolics-	P	0.9363	mg/l	3/19/2024 13:27:59	
P1788-02	S	Phenolics-	P	0.0058	mg/l	3/19/2024 13:37:50	
P1788-02DUP	S	Phenolics-	P	0.008	mg/l	3/19/2024 13:37:52	
P1788-01	S	Phenolics-	P	-2.156	mg/l	3/19/2024 14:00:35	
P1788-02MS	S	Phenolics-	P	0.9799	mg/l	3/19/2024 14:00:37	
P1788-02MSD	S	Phenolics-	P	0.9808	mg/l	3/19/2024 14:00:39	
CCV2	S	Phenolics-	P	0.9903	mg/l	3/19/2024 14:00:41	
CCB2	S	Phenolics-	P	0.0027	mg/l	3/19/2024 14:00:43	

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : 12

Instrument ID : Konelab

3/19/2024 13:03

Test Phenolics-


Accepted 3/19/2024 13:03

Factor 9.992

Bias 0.007

Coeff. of det. 0.999873

Errors

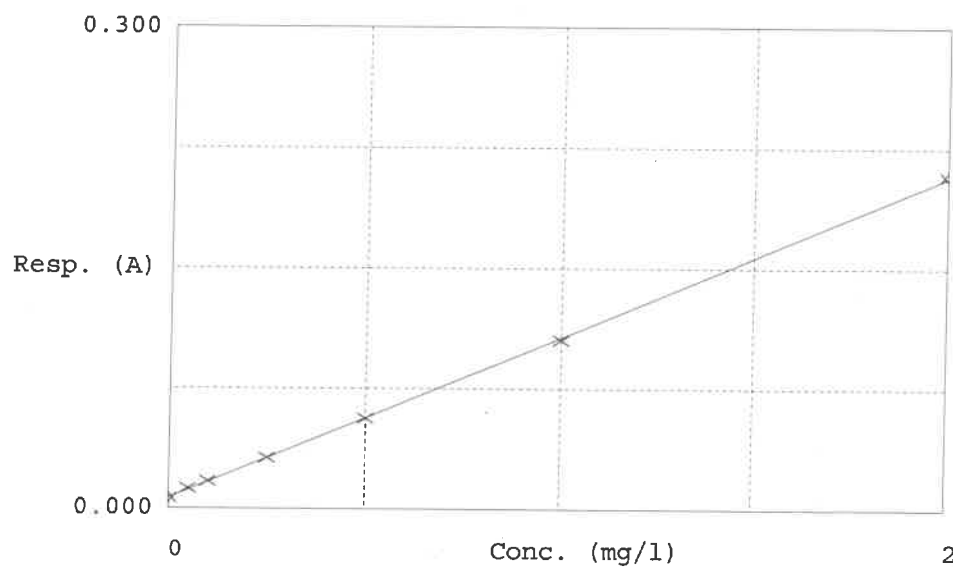

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.007	-0.0017	0.0000	-
2	Phenol-2	0.013	0.0591	0.0500	18.2
3	Phenol-2	0.017	0.1030	0.1000	3.0
4	Phenol-2	0.032	0.2500	0.2500	0.0
5	Phenol-2	0.056	0.4969	0.5000	-0.6
6	Phenol-2	0.105	0.9847	1.0000	-1.5
7	Phenol-2	0.208	2.0080	2.0000	0.4

12
3/19/24