


LB129991

7470A

INSTRUMENT ID: CV1

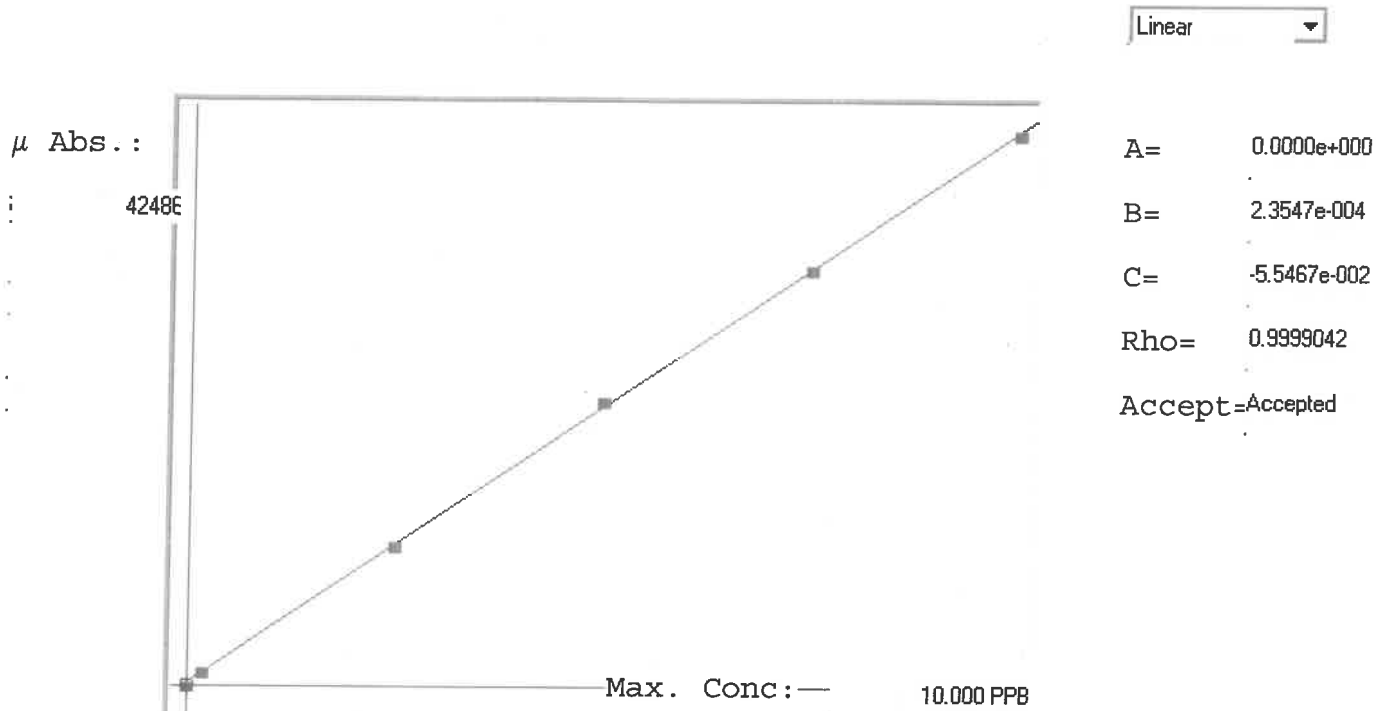

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.038	-0.038	74	0.000	74	0				
0.2	0.200	0.193	-0.007	1057	0.0 %	1057					
2.5	2.500	2.491	-0.009	10813	0.0 %	10813					
5.0	5.000	5.107	0.107	21924	0.0 %	21924					
7.5	7.500	7.499	-0.001	32081	0.0 %	32081					
10.0	10.000	9.949	-0.051	42486	0.0 %	42486					

=4
0
2
0
1

LB1299912 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 22 Mar 2024 09:02:06

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	74	-	0.0000	7470A	PPB	22 Mar 2024 09:06:14	S	Std
0.2 - 1	50.2	1057	-	0.2000	7470A	PPB	22 Mar 2024 09:08:31	S	Std
2.5 - 1	50.5	10813	-	2.5000	7470A	PPB	22 Mar 2024 09:10:49	S	Std
5.0 - 1	51	21924	-	5.0000	7470A	PPB	22 Mar 2024 09:13:06	S	Std
7.5 - 1	51.5	32081	-	7.5000	7470A	PPB	22 Mar 2024 09:15:24	S	Std
10.0 - 1	51.6	42486	-	10.0000	7470A	PPB	22 Mar 2024 09:20:28	S	Std
ICV59 - 1	ICV59	17692	4.1104	-	7470A	PPB	22 Mar 2024 09:23:47	U	SMPL
ICB59 - 1	ICB59	537	0.0710	-	7470A	PPB	22 Mar 2024 09:26:02	U	SMPL
CCV01 - 1	CCV01	20009	4.6560	-	7470A	PPB	22 Mar 2024 09:28:20	U	SMPL
CCB01 - 1	CCB01	495	0.0611	-	7470A	PPB	22 Mar 2024 09:30:35	U	SMPL
CRA - 1	CRA	999	0.1798	-	7470A	PPB	22 Mar 2024 09:32:52	U	SMPL
HighStd - 1	HighStd	42673	9.9926	-	7470A	PPB	22 Mar 2024 09:35:07	U	SMPL
ChkStd - 1	ChkStd	29164	6.8117	-	7470A	PPB	22 Mar 2024 09:37:22	U	SMPL
PB159728BL - 1	PBW	293	0.0135	-	7470A	PPB	22 Mar 2024 09:43:02	U	SMPL
PB159728BS - 1	LCSW	15001	3.4768	-	7470A	PPB	22 Mar 2024 09:45:17	U	SMPL
P1798-01 - 1	S-1	23	-0.0501	-	7470A	PPB	22 Mar 2024 09:47:33	U	SMPL
P1798-02 - 1	S-2	13	-0.0524	-	7470A	PPB	22 Mar 2024 09:49:52	U	SMPL
P1798-03 - 1	S-3	454	0.0514	-	7470A	PPB	22 Mar 2024 09:52:09	U	SMPL
P1798-04 - 1	S-4	97	-0.0326	-	7470A	PPB	22 Mar 2024 09:54:26	U	SMPL
P1798-05 - 1	S-5	106	-0.0305	-	7470A	PPB	22 Mar 2024 09:56:41	U	SMPL
CCV02 - 1	CCV02	20272	4.7179	-	7470A	PPB	22 Mar 2024 09:58:57	U	SMPL
CCB02 - 1	CCB02	478	0.0571	-	7470A	PPB	22 Mar 2024 10:01:12	U	SMPL
P1798-06 - 1	S-6	134	-0.0239	-	7470A	PPB	22 Mar 2024 10:03:30	U	SMPL
P1798-07 - 1	S-7	169	-0.0157	-	7470A	PPB	22 Mar 2024 10:05:45	U	SMPL
P1798-08 - 1	S-8	218	-0.0041	-	7470A	PPB	22 Mar 2024 10:08:00	U	SMPL
P1798-09 - 1	S-9	130	-0.0249	-	7470A	PPB	22 Mar 2024 10:10:16	U	SMPL
P1798-10 - 1	S-10	191	-0.0105	-	7470A	PPB	22 Mar 2024 10:12:32	U	SMPL
P1798-11 - 1	S-11	131	-0.0246	-	7470A	PPB	22 Mar 2024 10:14:48	U	SMPL
P1798-12 - 1	S-12	140	-0.0225	-	7470A	PPB	22 Mar 2024 10:17:04	U	SMPL
P1798-13 - 1	S-13	162	-0.0173	-	7470A	PPB	22 Mar 2024 10:19:22	U	SMPL
P1798-14 - 1	S-14	159	-0.0180	-	7470A	PPB	22 Mar 2024 10:21:38	U	SMPL
P1798-15 - 1	S-15	170	-0.0154	-	7470A	PPB	22 Mar 2024 10:23:54	U	SMPL
CCV03 - 1	CCV03	20589	4.7926	-	7470A	PPB	22 Mar 2024 10:26:10	U	SMPL
CCB03 - 1	CCB03	629	0.0926	-	7470A	PPB	22 Mar 2024 10:28:25	U	SMPL
P1803-02 - 1	TRENCH-PIT	40	-0.0460	-	7470A	PPB	22 Mar 2024 10:30:43	U	SMPL
P1807-01 - 1	3461	2100	0.4390	-	7470A	PPB	22 Mar 2024 10:32:59	U	SMPL
P1807-02 - 1	3443	-261	-0.1169	-	7470A	PPB	22 Mar 2024 10:35:15	U	SMPL
P1807-03 - 1	3436-37	56	-0.0423	-	7470A	PPB	22 Mar 2024 10:37:32	U	SMPL
P1807-04 - 1	3450-59	61	-0.0411	-	7470A	PPB	22 Mar 2024 10:39:48	U	SMPL
P1807-04DUP - 1	3450-59DUP	24	-0.0498	-	7470A	PPB	22 Mar 2024 10:42:05	U	SMPL
P1807-04MS - 1	3450-59MS	16927	3.9303	-	7470A	PPB	22 Mar 2024 10:44:21	U	SMPL
P1807-04MSD - 1	3450-59MSD	16017	3.7160	-	7470A	PPB	22 Mar 2024 10:46:38	U	SMPL
PB159729BL - 1	PBW	-109	-0.0811	-	7470A	PPB	22 Mar 2024 10:48:57	U	SMPL
PB159729BS - 1	LCSW	15626	3.6239	-	7470A	PPB	22 Mar 2024 10:51:15	U	SMPL
CCV04 - 1	CCV04	19919	4.6348	-	7470A	PPB	22 Mar 2024 10:53:31	U	SMPL
CCB04 - 1	CCB04	573	0.0795	-	7470A	PPB	22 Mar 2024 10:55:48	U	SMPL
P1807-05 - 1	3462	160	-0.0178	-	7470A	PPB	22 Mar 2024 10:58:06	U	SMPL
P1807-05DUP - 1	3462DUP	170	-0.0154	-	7470A	PPB	22 Mar 2024 11:00:22	U	SMPL
P1807-05MS - 1	3462MS	15417	3.5747	-	7470A	PPB	22 Mar 2024 11:02:38	U	SMPL
P1807-05MSD - 1	3462MSD	14310	3.3141	-	7470A	PPB	22 Mar 2024 11:04:53	U	SMPL
PB159730BL - 1	PBW	287	0.0121	-	7470A	PPB	22 Mar 2024 11:10:15	U	SMPL
PB159730BS - 1	LCSW	18277	4.2482	-	7470A	PPB	22 Mar 2024 11:15:10	U	SMPL
P1800-01 - 1	1394	92	-0.0338	-	7470A	PPB	22 Mar 2024 11:17:26	U	SMPL
P1820-01 - 1	WASTE-WATER	1540	0.3072	-	7470A	PPB	22 Mar 2024 11:24:41	U	SMPL
P1820-01DUP - 1	WASTE-WATERDUP	1441	0.2838	-	7470A	PPB	22 Mar 2024 11:29:44	U	SMPL
P1820-01MS - 1	WASTE-WATERMS	17042	3.9574	-	7470A	PPB	22 Mar 2024 11:32:00	U	SMPL
CCV05 - 1	CCV05	19959	4.6442	-	7470A	PPB	22 Mar 2024 11:34:15	U	SMPL
CCB05 - 1	CCB05	490	0.0599	-	7470A	PPB	22 Mar 2024 11:36:33	U	SMPL
P1820-01MSD - 1	WASTE-WATERMSD	20363	4.7393	-	7470A	PPB	22 Mar 2024 11:38:51	U	SMPL
P1828-04 - 1	TRE-1290	274	0.0091	-	7470A	PPB	22 Mar 2024 11:41:07	U	SMPL
PB159676TB - 1	PB159676TB	46	-0.0446	-	7470A	PPB	22 Mar 2024 11:43:26	U	SMPL
PB159689TB - 1	PB159689TB	43	-0.0453	-	7470A	PPB	22 Mar 2024 11:45:41	U	SMPL
P1807-04LX5 - 1		47	-0.0444	-	7470A	PPB	22 Mar 2024 11:47:58	U	SMPL
P1807-04A - 1		16467	3.8220	-	7470A	PPB	22 Mar 2024 11:50:14	U	SMPL
P1807-05LX5 - 1		12	-0.0526	-	7470A	PPB	22 Mar 2024 11:52:31	U	SMPL
P1807-05A - 1		19299	4.4888	-	7470A	PPB	22 Mar 2024 11:54:50	U	SMPL
P1820-01LX5 - 1		127	-0.0256	-	7470A	PPB	22 Mar 2024 11:57:07	U	SMPL
P1820-01A - 1		19429	4.5194	-	7470A	PPB	22 Mar 2024 11:59:25	U	SMPL
CCV06 - 1	CCV06	20626	4.8013	-	7470A	PPB	22 Mar 2024 12:01:41	U	SMPL
CCB06 - 1	CCB06	626	0.0919	-	7470A	PPB	22 Mar 2024 12:04:00	U	SMPL