


LB130008

7471B

INSTRUMENT ID: CV4

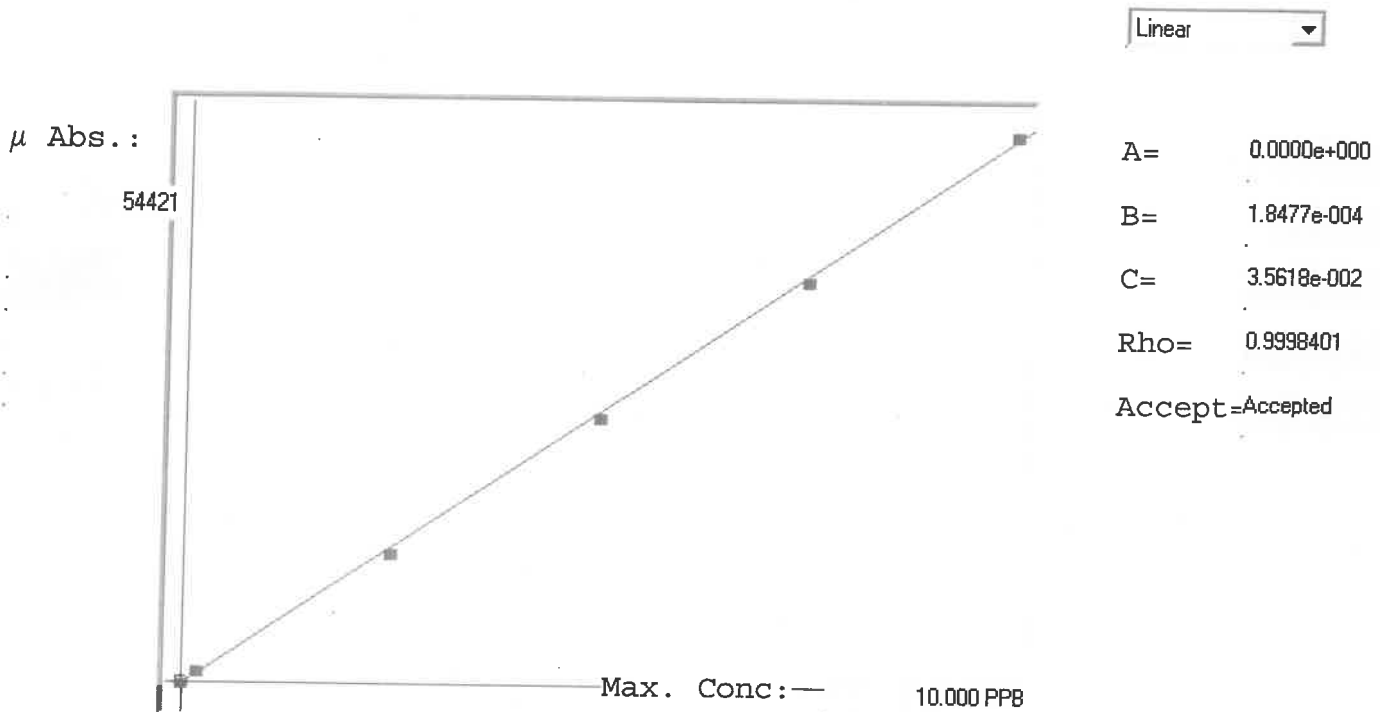

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%SD
0.0	0.000	0.058	0.058	121	0.000	121					
0.2	0.200	0.245	0.045	1131	0.0 %	1131					23
2.5	2.500	2.429	-0.071	12952	0.0 %	12952					3
5.0	5.000	4.940	-0.060	26542	0.0 %	26542					1
7.5	7.500	7.438	-0.062	40065	0.0 %	40065					1
10.0	10.000	10.091	0.091	54421	0.0 %	54421					1

LB130008 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 22 Mar 2024 16:08:37

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	121	-	0.0000	7471B	PPB	22 Mar 2024 16:13:31	S	Std
0.2 - 1	50.2	1131	-	0.2000	7471B	PPB	22 Mar 2024 16:15:49	S	Std
2.5 - 1	52.5	12952	-	2.5000	7471B	PPB	22 Mar 2024 16:18:06	S	Std
5.0 - 1	55	26542	-	5.0000	7471B	PPB	22 Mar 2024 16:20:23	S	Std
7.5 - 1	57.5	40065	-	7.5000	7471B	PPB	22 Mar 2024 16:22:43	S	Std
10.0 - 1	510	54421	-	10.0000	7471B	PPB	22 Mar 2024 16:27:46	S	Std
ICV61 - 1	ICV61	20824	3.8832	-	7471B	PPB	22 Mar 2024 16:33:50	U	SMPL
ICB61 - 1	ICB61	-4	0.0349	-	7471B	PPB	22 Mar 2024 16:36:07	U	SMPL
CCV09 - 1	CCV09	26725	4.9735	-	7471B	PPB	22 Mar 2024 16:38:25	U	SMPL
CCB09 - 1	CCB09	-89	0.0192	-	7471B	PPB	22 Mar 2024 16:40:40	U	SMPL
CRA - 1	CRA	1096	0.2381	-	7471B	PPB	22 Mar 2024 16:43:01	U	SMPL
HighStd - 1	HighStd	53240	9.8726	-	7471B	PPB	22 Mar 2024 16:45:16	U	SMPL
ChkStd - 1	ChkStd	37440	6.9533	-	7471B	PPB	22 Mar 2024 16:47:32	U	SMPL
PB159751BL - 1	PBS	-47	0.0269	-	7471B	PPB	22 Mar 2024 16:49:57	U	SMPL
PB159751BS - 1	LCSS	20194	3.7668	-	7471B	PPB	22 Mar 2024 16:52:20	U	SMPL
P1827-01 - 1	72-11933	6673	1.2686	-	7471B	PPB	22 Mar 2024 16:59:43	U	SMPL
P1827-01DUP - 1	72-11933DUP	6458	1.2288	-	7471B	PPB	22 Mar 2024 17:01:59	U	SMPL
P1827-01MS - 1	72-11933MS	27107	5.0441	-	7471B	PPB	22 Mar 2024 17:04:18	U	SMPL
P1827-01MSD - 1	72-11933MSD	25606	4.7667	-	7471B	PPB	22 Mar 2024 17:06:37	U	SMPL
P1829-01 - 1	TR-05-031224	536	0.1347	-	7471B	PPB	22 Mar 2024 17:08:58	U	SMPL
CCV10 - 1	CCV10	26305	4.8959	-	7471B	PPB	22 Mar 2024 17:11:18	U	SMPL
CCB10 - 1	CCB10	-75	0.0218	-	7471B	PPB	22 Mar 2024 17:13:33	U	SMPL
P1830-02 - 1	VNJ-206	2756	0.5448	-	7471B	PPB	22 Mar 2024 17:15:52	U	SMPL
P1830-04 - 1	VNJ-226	9071	1.7116	-	7471B	PPB	22 Mar 2024 17:18:07	U	SMPL
P1831-01 - 1	CL-01-032124	13100	2.4561	-	7471B	PPB	22 Mar 2024 17:20:24	U	SMPL
P1832-01 - 1	600581536	1216	0.2603	-	7471B	PPB	22 Mar 2024 17:22:42	U	SMPL
P1827-01LX5 - 1		1317	0.2790	-	7471B	PPB	22 Mar 2024 17:25:01	U	SMPL
P1827-01A - 1		27796	5.1714	-	7471B	PPB	22 Mar 2024 17:27:17	U	SMPL
CCV11 - 1	CCV11	26710	4.9707	-	7471B	PPB	22 Mar 2024 17:29:33	U	SMPL
CCB11 - 1	CCB11	74	0.0493	-	7471B	PPB	22 Mar 2024 17:31:55	U	SMPL