


LB130129
~~LB130023~~

7470A INSTRUMENT ID: CVJ

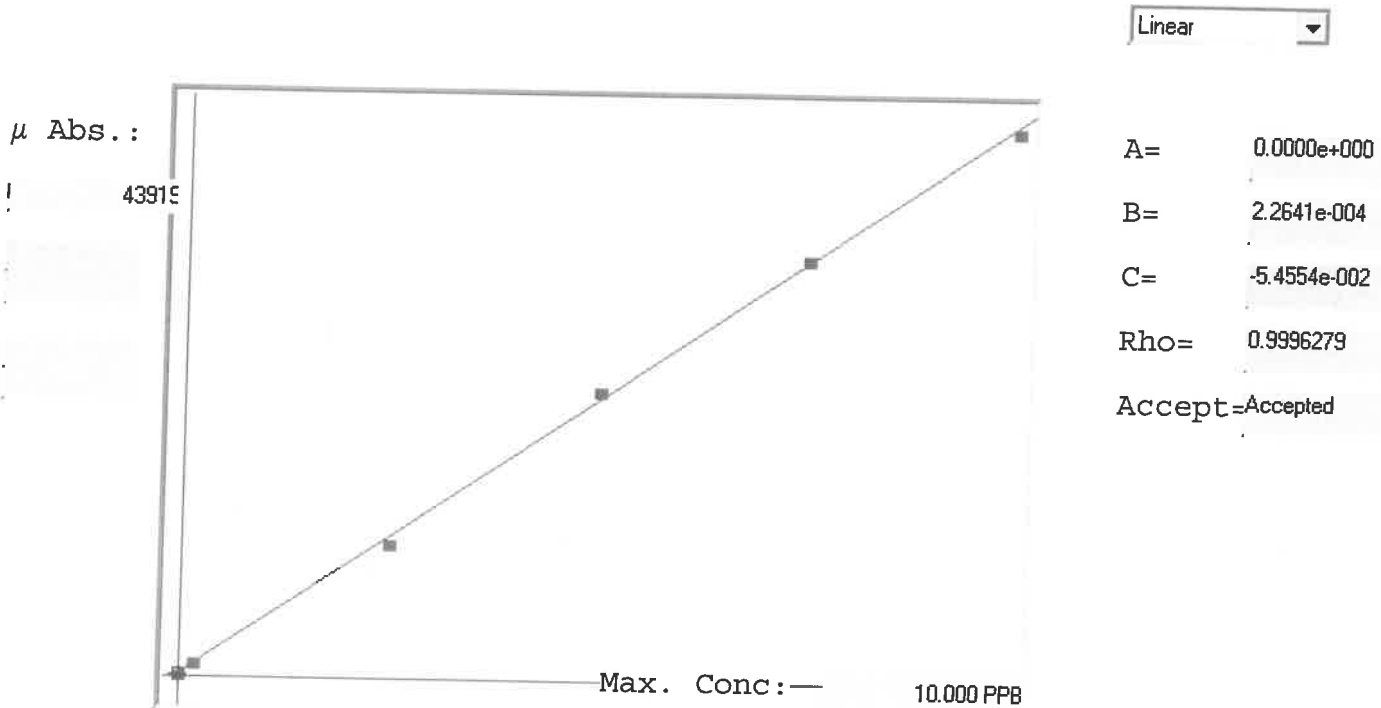

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/0/1
0.0	0.000	-0.011	-0.011	193	0.000	193					
0.2	0.200	0.208	0.008	1160	0.0 %	1160	0				4
2.5	2.500	2.377	-0.123	10739	0.0 %	10739					-5
5.0	5.000	5.169	0.169	23070	0.0 %	23070					3
7.5	7.500	7.568	0.068	33669	0.0 %	33669					1
10.0	10.000	9.889	-0.111	43919	0.0 %	43919					-1

LB130129

LB43023 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 02 Apr 2024 11:11:16

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	S0	193	-	0.0000	7470A	PPB	02 Apr 2024 11:24:39	S	Std
0.2 - 1	S0.2	1160	-	0.2000	7470A	PPB	02 Apr 2024 11:26:57	S	Std
2.5 - 1	S2.5	10739	-	2.5000	7470A	PPB	02 Apr 2024 11:29:14	S	Std
5.0 - 1	S5	23070	-	5.0000	7470A	PPB	02 Apr 2024 11:31:31	S	Std
7.5 - 1	S7.5	33669	-	7.5000	7470A	PPB	02 Apr 2024 11:40:03	S	Std
10.0 - 1	S10	43919	-	10.0000	7470A	PPB	02 Apr 2024 11:47:43	S	Std
ICV73 - 1	ICV73	18320	4.0932	-	7470A	PPB	02 Apr 2024 11:50:30	U	SMPL
ICB73 - 1	ICB73	-125	-0.0829	-	7470A	PPB	02 Apr 2024 11:52:45	U	SMPL
CCV46 - 1	CCV46	23844	5.3439	-	7470A	PPB	02 Apr 2024 11:55:03	U	SMPL
CCB46 - 1	CCB46	-171	-0.0933	-	7470A	PPB	02 Apr 2024 11:57:17	U	SMPL
CRA - 1	CRA	998	0.1714	-	7470A	PPB	02 Apr 2024 11:59:35	U	SMPL
HighStd - 1	HighStd	44049	9.9184	-	7470A	PPB	02 Apr 2024 12:01:50	U	SMPL
ChkStd - 1	ChkStd	29620	6.6516	-	7470A	PPB	02 Apr 2024 12:04:06	U	SMPL
PB159899BL - 1	PBW	53	-0.0426	-	7470A	PPB	02 Apr 2024 12:08:58	U	SMPL
PB159899BS - 1	LCSW	19905	4.4521	-	7470A	PPB	02 Apr 2024 12:13:54	U	SMPL
P1915-02 - 1	WC-A-COMP	-108	-0.0790	-	7470A	PPB	02 Apr 2024 12:16:10	U	SMPL
P1915-02DUP - 1	WC-A-COMPDUP	56	-0.0419	-	7470A	PPB	02 Apr 2024 12:18:29	U	SMPL
P1915-02MS - 1	WC-A-COMPMS	18178	4.0611	-	7470A	PPB	02 Apr 2024 12:23:20	U	SMPL
P1915-02MSD - 1	WC-A-COMPMSD	18622	4.1616	-	7470A	PPB	02 Apr 2024 12:29:30	U	SMPL
P1921-01 - 1	S-16	24	-0.0491	-	7470A	PPB	02 Apr 2024 12:31:45	U	SMPL
CCV47 - 1	CCV47	22705	5.0860	-	7470A	PPB	02 Apr 2024 12:34:02	U	SMPL
CCB47 - 1	CCB47	-120	-0.0817	-	7470A	PPB	02 Apr 2024 12:36:18	U	SMPL
P1921-02 - 1	S-17	86	-0.0351	-	7470A	PPB	02 Apr 2024 12:38:35	U	SMPL
P1921-03 - 1	S-18	144	-0.0220	-	7470A	PPB	02 Apr 2024 12:40:50	U	SMPL
P1921-04 - 1	S-19	1296	0.2389	-	7470A	PPB	02 Apr 2024 12:43:06	U	SMPL
P1921-05 - 1	S-20	-46	-0.0650	-	7470A	PPB	02 Apr 2024 12:45:22	U	SMPL
P1921-06 - 1	S-21	103	-0.0312	-	7470A	PPB	02 Apr 2024 12:47:40	U	SMPL
P1921-07 - 1	S-22	116	-0.0283	-	7470A	PPB	02 Apr 2024 12:49:56	U	SMPL
PB159900BL - 1	PBW	116	-0.0283	-	7470A	PPB	02 Apr 2024 12:52:12	U	SMPL
PB159900BS - 1	LCSW	15130	3.3710	-	7470A	PPB	02 Apr 2024 12:54:29	U	SMPL
P1927-02 - 1	72-11991	-37	-0.0629	-	7470A	PPB	02 Apr 2024 12:56:46	U	SMPL
P1927-02DUP - 1	72-11991DUP	164	-0.0174	-	7470A	PPB	02 Apr 2024 12:59:04	U	SMPL
CCV48 - 1	CCV48	23300	5.2207	-	7470A	PPB	02 Apr 2024 13:01:20	U	SMPL
CCB48 - 1	CCB48	-159	-0.0906	-	7470A	PPB	02 Apr 2024 13:03:36	U	SMPL
P1927-02MS - 1	72-11991MS	19702	4.4061	-	7470A	PPB	02 Apr 2024 13:05:54	U	SMPL
P1927-02MSD - 1	72-11991MSD	19313	4.3180	-	7470A	PPB	02 Apr 2024 13:08:09	U	SMPL
P1927-04 - 1	72-11998	190	-0.0115	-	7470A	PPB	02 Apr 2024 13:10:27	U	SMPL
P1935-02 - 1	TPMH	290	0.0111	-	7470A	PPB	02 Apr 2024 13:12:45	U	SMPL
PB159933BL - 1	PBW	247	0.0014	-	7470A	PPB	02 Apr 2024 13:15:01	U	SMPL
PB159933BS - 1	LCSW	19138	4.2784	-	7470A	PPB	02 Apr 2024 13:17:17	U	SMPL
P1935-03 - 1	BELL-TOTES	-42	-0.0641	-	7470A	PPB	02 Apr 2024 13:19:34	U	SMPL
P1937-01 - 1	A5552	220	-0.0047	-	7470A	PPB	02 Apr 2024 13:21:53	U	SMPL
P1937-01DUP - 1	A5552DUP	345	0.0236	-	7470A	PPB	02 Apr 2024 13:24:10	U	SMPL
P1937-01MS - 1	A5552MS	17940	4.0072	-	7470A	PPB	02 Apr 2024 13:26:26	U	SMPL
CCV49 - 1	CCV49	22110	4.9513	-	7470A	PPB	02 Apr 2024 13:28:41	U	SMPL
CCB49 - 1	CCB49	121	-0.0272	-	7470A	PPB	02 Apr 2024 13:34:17	U	SMPL
P1937-01MSD - 1	A5552MSD	17730	3.9596	-	7470A	PPB	02 Apr 2024 13:36:33	U	SMPL
PB159858TB - 1	PB159858TB	121	-0.0272	-	7470A	PPB	02 Apr 2024 13:41:34	U	SMPL
PB159890TB - 1	PB159890TB	168	-0.0165	-	7470A	PPB	02 Apr 2024 13:43:49	U	SMPL
P1915-02LX5 - 1		14	-0.0514	-	7470A	PPB	02 Apr 2024 13:46:05	U	SMPL
P1915-02A - 1		19043	4.2569	-	7470A	PPB	02 Apr 2024 13:48:20	U	SMPL
P1927-02LX5 - 1		-84	-0.0736	-	7470A	PPB	02 Apr 2024 13:50:37	U	SMPL
P1927-02A - 1		18973	4.2411	-	7470A	PPB	02 Apr 2024 13:52:55	U	SMPL
P1937-01LX5 - 1		-154	-0.0894	-	7470A	PPB	02 Apr 2024 13:55:12	U	SMPL
P1937-01A - 1		18923	4.2297	-	7470A	PPB	02 Apr 2024 13:57:31	U	SMPL
CCV50 - 1	CCV50	22220	4.9762	-	7470A	PPB	02 Apr 2024 13:59:47	U	SMPL
CCB50 - 1	CCB50	-101	-0.0774	-	7470A	PPB	02 Apr 2024 14:02:06	U	SMPL