


LB130169

7470A

INSTRUMENT ID: V1

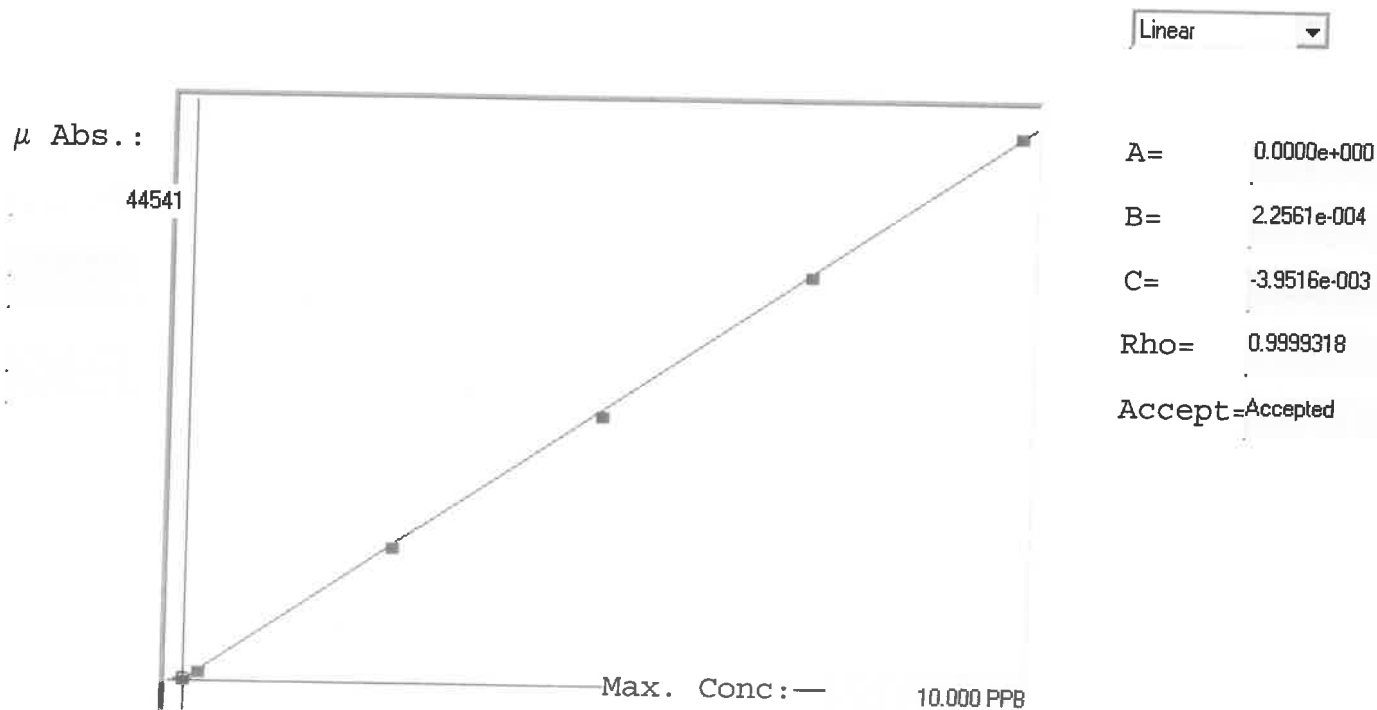

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.051	0.051	243	0.000	243					
0.2	0.200	0.199	-0.001	900	0.0 %	900	0				-1
2.5	2.500	2.490	-0.010	11053	0.0 %	11053					0
5.0	5.000	4.920	-0.080	21825	0.0 %	21825					2
7.5	7.500	7.495	-0.005	33240	0.0 %	33240					0
10.0	10.000	10.045	0.045	44541	0.0 %	44541					0

LB130169 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 04 Apr 2024 12:32:58

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	243	-	0.0000	7470A	PPB	04 Apr 2024 12:42:20	S	Std
0.2 - 1	50-2	900	-	0.2000	7470A	PPB	04 Apr 2024 12:44:37	S	Std
2.5 - 1	52.5	11053	-	2.5000	7470A	PPB	04 Apr 2024 12:46:54	S	Std
5.0 - 1	55	21825	-	5.0000	7470A	PPB	04 Apr 2024 12:49:11	S	Std
7.5 - 1	57.5	33240	-	7.5000	7470A	PPB	04 Apr 2024 12:51:29	S	Std
10.0 - 1	5/1	44541	-	10.0000	7470A	PPB	04 Apr 2024 12:59:26	S	Std
ICV79 - 1	ICV79	16986	3.8283	-	7470A	PPB	04 Apr 2024 13:02:11	U	SMPL
ICB79 - 1	ICB79	75	0.0130	-	7470A	PPB	04 Apr 2024 13:04:28	U	SMPL
CCV62 - 1	CCV62	23029	5.1916	-	7470A	PPB	04 Apr 2024 13:06:46	U	SMPL
CCB62 - 1	CCB62	62	0.0100	-	7470A	PPB	04 Apr 2024 13:09:01	U	SMPL
CRA - 1	CRA	897	0.1984	-	7470A	PPB	04 Apr 2024 13:11:19	U	SMPL
HighStd - 1	HighStd	44291	9.9886	-	7470A	PPB	04 Apr 2024 13:13:34	U	SMPL
ChkStd - 1	ChkStd	31737	7.1563	-	7470A	PPB	04 Apr 2024 13:15:49	U	SMPL
PB159985BL - 1	PBW	-305	-0.0728	-	7470A	PPB	04 Apr 2024 13:18:10	U	SMPL
PB159985BS - 1	LCSW	17624	3.9722	-	7470A	PPB	04 Apr 2024 13:20:28	U	SMPL
P1945-01 - 1	SEW-10	830	0.1833	-	7470A	PPB	04 Apr 2024 13:34:57	U	SMPL
P1945-01DUP - 1	SEW-10DUP	712	0.1567	-	7470A	PPB	04 Apr 2024 13:37:13	U	SMPL
P1945-01MS - 1	SEW-10MS	18198	4.1017	-	7470A	PPB	04 Apr 2024 13:39:30	U	SMPL
P1945-01MSD - 1	SEW-10MSD	17690	3.9871	-	7470A	PPB	04 Apr 2024 13:41:47	U	SMPL
P1945-02 - 1	SEW-11	347	0.0743	-	7470A	PPB	04 Apr 2024 13:44:05	U	SMPL
CCV63 - 1	CCV63	23935	5.3960	-	7470A	PPB	04 Apr 2024 13:46:23	U	SMPL
CCB63 - 1	CCB63	119	0.0229	-	7470A	PPB	04 Apr 2024 13:48:38	U	SMPL
P1956-02 - 1	231	457	0.0992	-	7470A	PPB	04 Apr 2024 13:50:57	U	SMPL
P1956-03 - 1	236	490	0.1066	-	7470A	PPB	04 Apr 2024 13:53:12	U	SMPL
P1957-02 - 1	NM-DRUMS-040224	400	0.0863	-	7470A	PPB	04 Apr 2024 13:55:28	U	SMPL
P1960-01 - 1	3471	484	0.1052	-	7470A	PPB	04 Apr 2024 13:57:43	U	SMPL
P1963-01 - 1	391	415	0.0897	-	7470A	PPB	04 Apr 2024 13:59:59	U	SMPL
PB159986BL - 1	PBW	424	0.0917	-	7470A	PPB	04 Apr 2024 14:02:15	U	SMPL
PB159986BS - 1	LCSW	15941	3.5925	-	7470A	PPB	04 Apr 2024 14:04:32	U	SMPL
P1956-01 - 1	232	201	0.0414	-	7470A	PPB	04 Apr 2024 14:06:49	U	SMPL
P1956-01DUP - 1	232DUP	-28	-0.0103	-	7470A	PPB	04 Apr 2024 14:09:14	U	SMPL
P1956-01MS - 1	232MS	17352	3.9108	-	7470A	PPB	04 Apr 2024 14:22:06	U	SMPL
CCV64 - 1	CCV64	21806	4.9157	-	7470A	PPB	04 Apr 2024 14:24:22	U	SMPL
CCB64 - 1	CCB64	222	0.0461	-	7470A	PPB	04 Apr 2024 14:26:40	U	SMPL
P1956-01MSD - 1	232MSD	16952	3.8206	-	7470A	PPB	04 Apr 2024 14:31:32	U	SMPL
PB159944TB - 1	PB159944TB	115	0.0220	-	7470A	PPB	04 Apr 2024 14:33:48	U	SMPL
PB159961TB - 1	PB159961TB	345	0.0739	-	7470A	PPB	04 Apr 2024 14:36:06	U	SMPL
P1945-01LX5 - 1		27	0.0021	-	7470A	PPB	04 Apr 2024 14:38:22	U	SMPL
P1945-01A - 1		17902	4.0349	-	7470A	PPB	04 Apr 2024 14:40:38	U	SMPL
P1956-01LX5 - 1		-106	-0.0279	-	7470A	PPB	04 Apr 2024 14:42:55	U	SMPL
P1956-01A - 1		16819	3.7906	-	7470A	PPB	04 Apr 2024 14:45:14	U	SMPL
CCV65 - 1	CCV65	23849	5.3766	-	7470A	PPB	04 Apr 2024 14:58:14	U	SMPL
CCB65 - 1	CCB65	2	-0.0035	-	7470A	PPB	04 Apr 2024 15:00:31	U	SMPL