


LB130183

SFAM01.1 INSTRUMENT ID: CV1

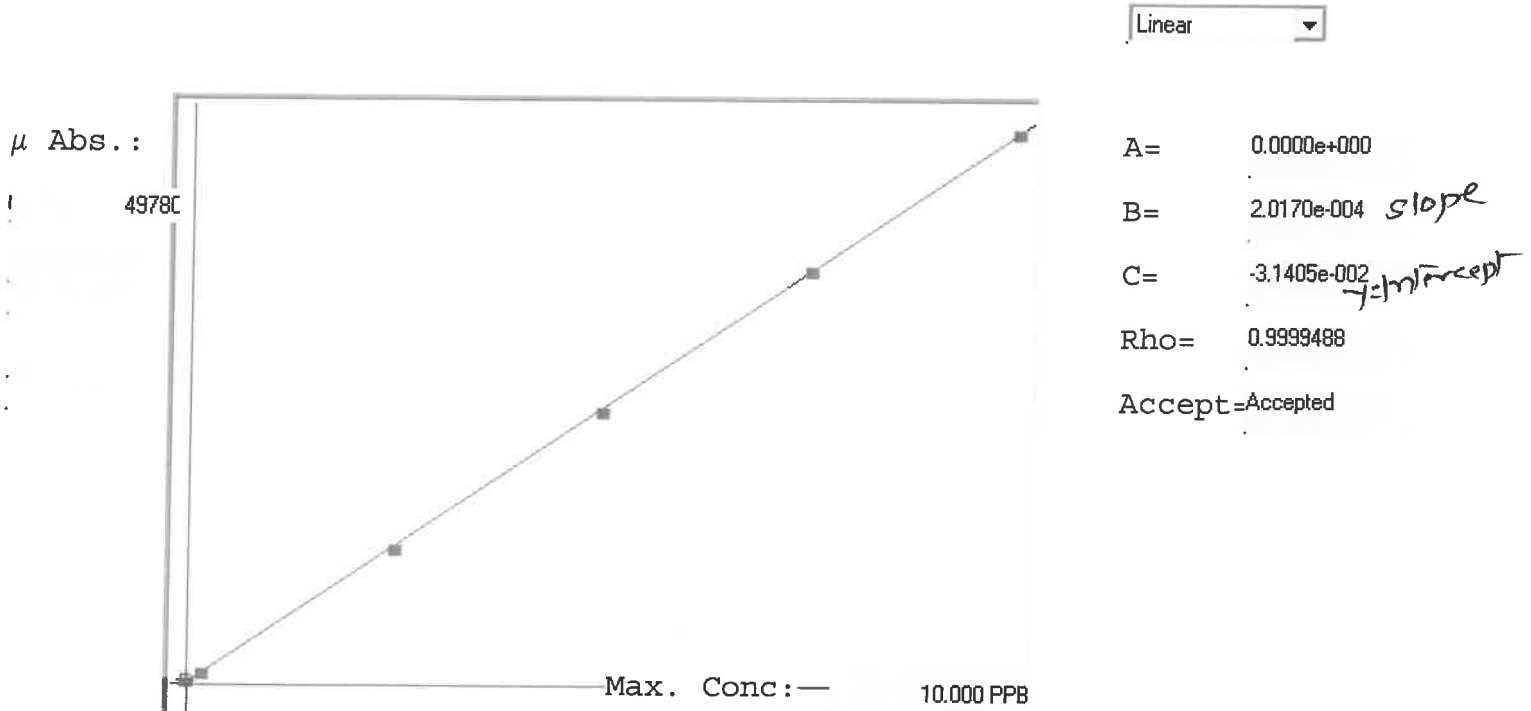

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/a)
0.00	0.000	0.053	0.053	416	0.000	416					=
0.05	0.050					442	0				-1
0.20	0.200	0.198	-0.002	1137	0.0 %	1137					-2
2.50	2.500	2.455	-0.045	12326	0.0 %	12326					-1
5.00	5.000	4.952	-0.048	24705	0.0 %	24705					0
7.50	7.500	7.534	0.034	37506	0.0 %	37506					0
10.0	10.000	10.009	0.009	49780	0.0 %	49780					0

LB130183

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0	416	-		0 SFAM01.1	PPB	4/4/2024 18:23	Std
	0.2	1137	-		0.2 SFAM01.1	PPB	4/4/2024 18:26	Std
	2.5	12326	-		2.5 SFAM01.1	PPB	4/4/2024 18:28	Std
	5	24705	-		5 SFAM01.1	PPB	4/4/2024 18:30	Std
	7.5	37506	-		7.5 SFAM01.1	PPB	4/4/2024 18:33	Std
	10	49780	-		10 SFAM01.1	PPB	4/4/2024 18:35	Std
ICV081	ICV081	19483	3.8984 -		SFAM01.1	PPB	4/4/2024 18:38	SMPL
ICB081	ICB081	210	0.011 -		SFAM01.1	PPB	4/4/2024 18:40	SMPL
CCV070	CCV070	25040	5.0193 -		SFAM01.1	PPB	4/4/2024 18:42	SMPL
CCB070	CCB070	188	0.0065 -		SFAM01.1	PPB	4/4/2024 18:45	SMPL
PB160021BL	PBS002	357	0.0406 -		SFAM01.1	PPB	4/4/2024 18:47	SMPL
P1990-01	E07T3	4457	0.8676 -		SFAM01.1	PPB	4/4/2024 18:49	SMPL
P1990-02	E07T4	1255	0.2217 -		SFAM01.1	PPB	4/4/2024 18:51	SMPL
P1990-03	E07T5	825	0.135 -		SFAM01.1	PPB	4/4/2024 18:54	SMPL
P1990-04	E07T6	878	0.1457 -		SFAM01.1	PPB	4/4/2024 18:56	SMPL
P1990-05	E07T6D	789	0.1277 -		SFAM01.1	PPB	4/4/2024 18:58	SMPL
P1990-06	E07T6S	12761	2.5425 -		SFAM01.1	PPB	4/4/2024 19:00	SMPL
CCV071	CCV071	23892	4.7877 -		SFAM01.1	PPB	4/4/2024 19:03	SMPL
CCB071	CCB071	246	0.0182 -		SFAM01.1	PPB	4/4/2024 19:05	SMPL