


LB130222

7471B

INSTRUMENT ID: CV1

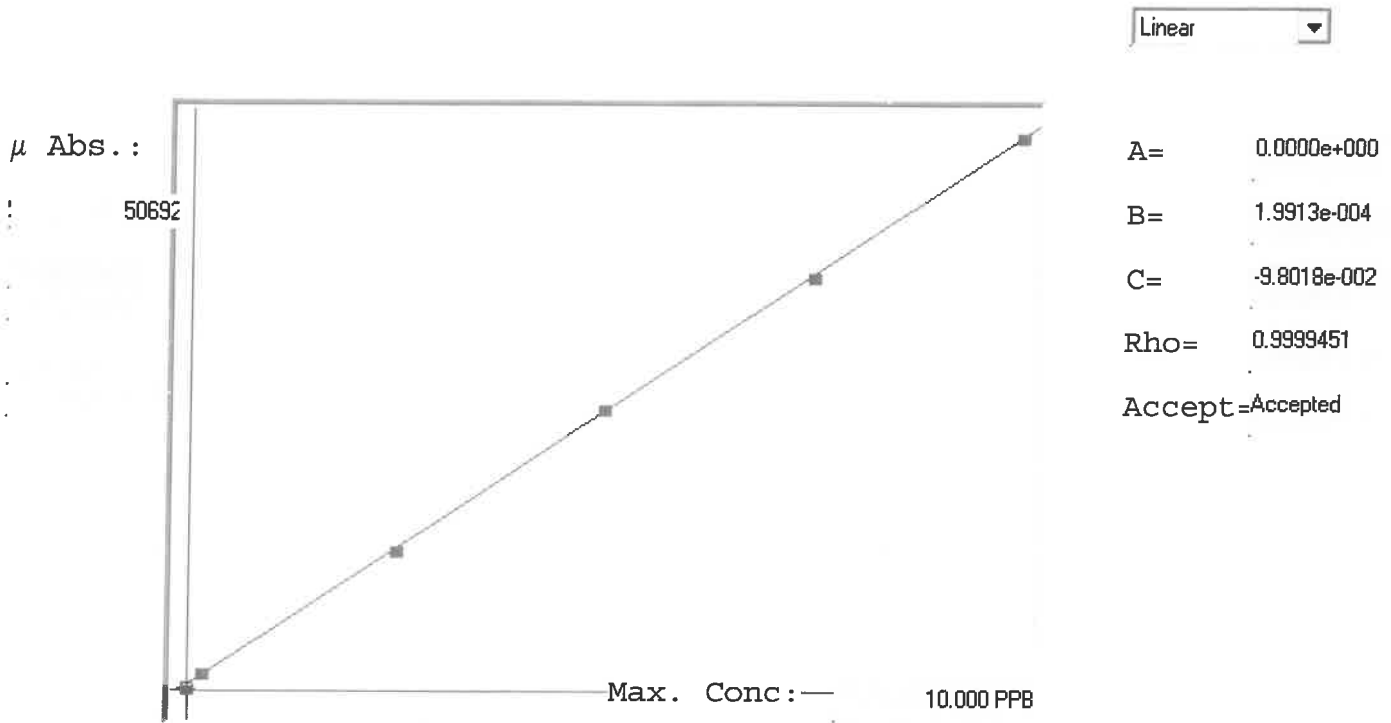

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%RSD
0.0	0.000	-0.036	-0.036	312	0.000	312					0
0.2	0.200	0.239	0.039	1695	0.0 %	1695					20
2.5	2.500	2.464	-0.036	12867	0.0 %	12867					1
5.0	5.000	5.064	0.064	25922	0.0 %	25922					1
7.5	7.500	7.473	-0.027	38019	0.0 %	38019					0
10.0	10.000	9.996	-0.004	50692	0.0 %	50692					0

LB130222 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 08 Apr 2024 16:23:30

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	312	-	0.0000	7471B	PPB	08 Apr 2024 16:29:53	S	Std
0.2 - 1	50.2	1695	-	0.2000	7471B	PPB	08 Apr 2024 16:32:10	S	Std
2.5 - 1	52.5	12867	-	2.5000	7471B	PPB	08 Apr 2024 16:34:28	S	Std
5.0 - 1	55	25922	-	5.0000	7471B	PPB	08 Apr 2024 16:36:45	S	Std
7.5 - 1	57.5	38019	-	7.5000	7471B	PPB	08 Apr 2024 16:39:04	S	Std
10.0 - 1	510	50692	-	10.0000	7471B	PPB	08 Apr 2024 16:41:28	S	Std
ICV87 - 1	ICV87	20297	3.9436	-	7471B	PPB	08 Apr 2024 16:44:56	U	SMPL
ICB87 - 1	ICB87	175	-0.0632	-	7471B	PPB	08 Apr 2024 16:47:12	U	SMPL
CCV89 - 1	CCV89	26478	5.1744	-	7471B	PPB	08 Apr 2024 16:49:34	U	SMPL
CCB89 - 1	CCB89	139	-0.0703	-	7471B	PPB	08 Apr 2024 16:51:50	U	SMPL
CRA - 1	CRA	1696	0.2397	-	7471B	PPB	08 Apr 2024 16:54:14	U	SMPL
HighStd - 1	HighStd	51572	10.1713	-	7471B	PPB	08 Apr 2024 16:56:29	U	SMPL
ChkStd - 1	ChkStd	36427	7.1555	-	7471B	PPB	08 Apr 2024 16:58:44	U	SMPL
PB160114BL - 1	PBS	486	-0.0012	-	7471B	PPB	08 Apr 2024 17:04:10	U	SMPL
PB160114BS - 1	LCSS	18287	3.5434	-	7471B	PPB	08 Apr 2024 17:06:26	U	SMPL
P1995-01 - 1	280648	16969	3.2809	-	7471B	PPB	08 Apr 2024 17:08:43	U	SMPL
P1995-03 - 1	MOO-23-00119	3580	0.6149	-	7471B	PPB	08 Apr 2024 17:11:05	U	SMPL
P1995-05 - 1	MOO-23-00113	1339	0.1686	-	7471B	PPB	08 Apr 2024 17:13:25	U	SMPL
P1995-05DUP - 1	MOO-23-00113DUP	853	0.0718	-	7471B	PPB	08 Apr 2024 17:15:43	U	SMPL
P1995-05MS - 1	MOO-23-00113MS	21215	4.1264	-	7471B	PPB	08 Apr 2024 17:28:06	U	SMPL
CCV90 - 1	CCV90	26043	5.0878	-	7471B	PPB	08 Apr 2024 17:30:21	U	SMPL
CCB90 - 1	CCB90	259	-0.0464	-	7471B	PPB	08 Apr 2024 17:32:42	U	SMPL
P1995-05MSD - 1	MOO-23-00113MSD	22990	4.4799	-	7471B	PPB	08 Apr 2024 17:35:04	U	SMPL
P1996-01 - 1	TP1	1365	0.1738	-	7471B	PPB	08 Apr 2024 17:37:20	U	SMPL
P1996-04 - 1	TP2	4899	0.8775	-	7471B	PPB	08 Apr 2024 17:39:42	U	SMPL
P1996-07 - 1	TP3	9073	1.7086	-	7471B	PPB	08 Apr 2024 17:41:59	U	SMPL
P1995-05LX5 - 1		1	-0.0978	-	7471B	PPB	08 Apr 2024 17:44:17	U	SMPL
P1995-05A - 1		22646	4.4114	-	7471B	PPB	08 Apr 2024 17:46:36	U	SMPL
CCV91 - 1	CCV91	27253	5.3287	-	7471B	PPB	08 Apr 2024 17:48:52	U	SMPL
CCB91 - 1	CCB91	261	-0.0460	-	7471B	PPB	08 Apr 2024 17:51:13	U	SMPL