


LB130257

7470A

INSTRUMENT ID: CV1

Linear

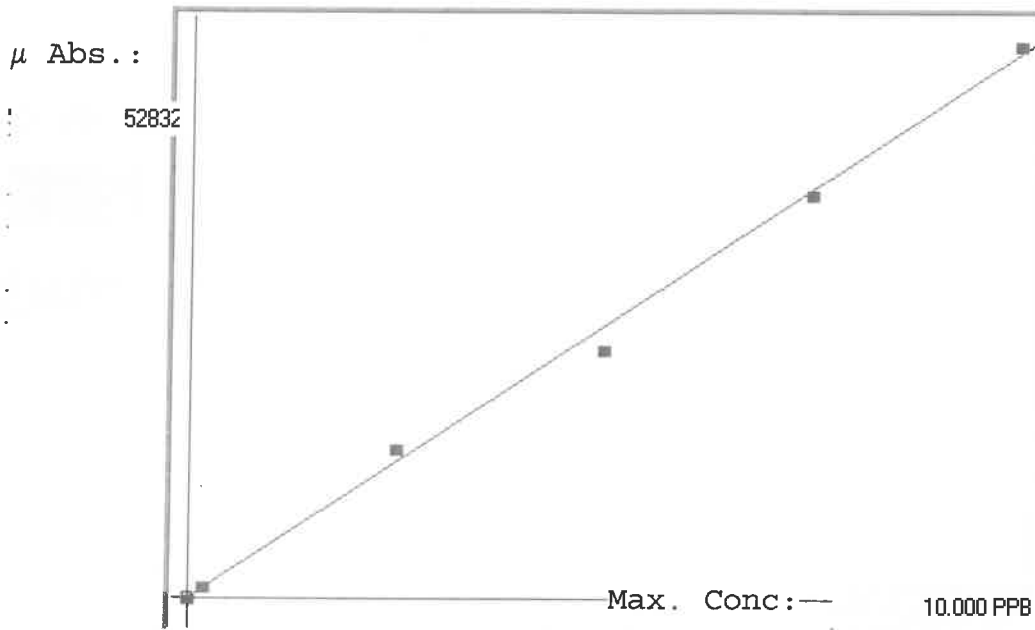

A= 0.0000e+000

B= 1.9214e-004

C= 4.6800e-003

Rho= 0.9984348

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/p
0.0	0.000	0.031	0.031	136	0.000	136	0				0/0
0.2	0.200	0.217	0.017	1105	0.0 %	1105					1
2.5	2.500	2.758	0.258	14329	0.0 %	14329					10
5.0	5.000	4.600	-0.400	23918	0.0 %	23918					10
7.5	7.500	7.438	-0.062	38690	0.0 %	38690					1
10.0	10.000	10.156	0.156	52832	0.0 %	52832					2

LB130257 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 10 Apr 2024 13:21:02

Sample ID	Extended ID	µ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	136	-	0.0000	7470A	PPB	10 Apr 2024 13:31:56	S	Std
0.2 - 1	50.2	1105	-	0.2000	7470A	PPB	10 Apr 2024 13:34:13	S	Std
2.5 - 1	52.5	14329	-	2.5000	7470A	PPB	10 Apr 2024 13:36:30	S	Std
5.0 - 1	55	23918	-	5.0000	7470A	PPB	10 Apr 2024 13:38:47	S	Std
7.5 - 1	57.5	38690	-	7.5000	7470A	PPB	10 Apr 2024 13:41:05	S	Std
10.0 - 1	511	52832	-	10.0000	7470A	PPB	10 Apr 2024 13:46:03	S	Std
ICV91 - 1	ICV91	19954	3.8386	-	7470A	PPB	10 Apr 2024 13:51:52	U	SMPL
ICB91 - 1	ICB91	-269	-0.0470	-	7470A	PPB	10 Apr 2024 13:54:08	U	SMPL
CCV01 - 1	CCV01	28473	5.4754	-	7470A	PPB	10 Apr 2024 13:56:25	U	SMPL
CCB01 - 1	CCB01	-247	-0.0428	-	7470A	PPB	10 Apr 2024 13:58:40	U	SMPL
CRA - 1	CRA	1029	0.2024	-	7470A	PPB	10 Apr 2024 14:00:59	U	SMPL
HighStd - 1	HighStd	52500	10.0919	-	7470A	PPB	10 Apr 2024 14:03:14	U	SMPL
ChkStd - 1	ChkStd	35667	6.8576	-	7470A	PPB	10 Apr 2024 14:05:30	U	SMPL
PB160156BL - 1	PBW	-542	-0.0995	-	7470A	PPB	10 Apr 2024 14:07:50	U	SMPL
PB160156BS - 1	LCSW	19361	3.7247	-	7470A	PPB	10 Apr 2024 14:10:08	U	SMPL
P1910-07 - 1	PT-HG-WP	127381	24.4793	-	7470A	PPB	10 Apr 2024 14:17:18	U	SMPL
P2019-01 - 1	NB205-WATER	4722	0.9120	-	7470A	PPB	10 Apr 2024 14:24:39	U	SMPL
P2019-01DUP - 1	NB205-WATERDUP	4492	0.8678	-	7470A	PPB	10 Apr 2024 14:35:12	U	SMPL
CCV02 - 1	CCV02	26692	5.1332	-	7470A	PPB	10 Apr 2024 14:37:28	U	SMPL
CCB02 - 1	CCB02	-6	0.0035	-	7470A	PPB	10 Apr 2024 14:39:45	U	SMPL
P2019-01MS - 1	NB205-WATERMS	23089	4.4409	-	7470A	PPB	10 Apr 2024 14:42:02	U	SMPL
P2019-01MSD - 1	NB205-WATERMSD	22183	4.2669	-	7470A	PPB	10 Apr 2024 14:44:17	U	SMPL
P2025-01 - 1	TOTE-COMP	40344	7.7563	-	7470A	PPB	10 Apr 2024 14:46:35	U	SMPL
P2025-03 - 1	TOTE-COMP	44350	8.5260	-	7470A	PPB	10 Apr 2024 14:48:53	U	SMPL
P2019-01LX5 - 1		766	0.1519	-	7470A	PPB	10 Apr 2024 14:51:12	U	SMPL
P2019-01A - 1		23006	4.4250	-	7470A	PPB	10 Apr 2024 14:53:31	U	SMPL
P1910-07DLX5 - 1	PT-HG-WP	27308	5.2516	-	7470A	PPB	10 Apr 2024 15:00:25	U	SMPL
CCV03 - 1	CCV03	27796	5.3453	-	7470A	PPB	10 Apr 2024 15:05:00	U	SMPL
CCB03 - 1	CCB03	-120	-0.0184	-	7470A	PPB	10 Apr 2024 15:07:18	U	SMPL