


LB130319

7470A

INSTRUMENT ID: CV1

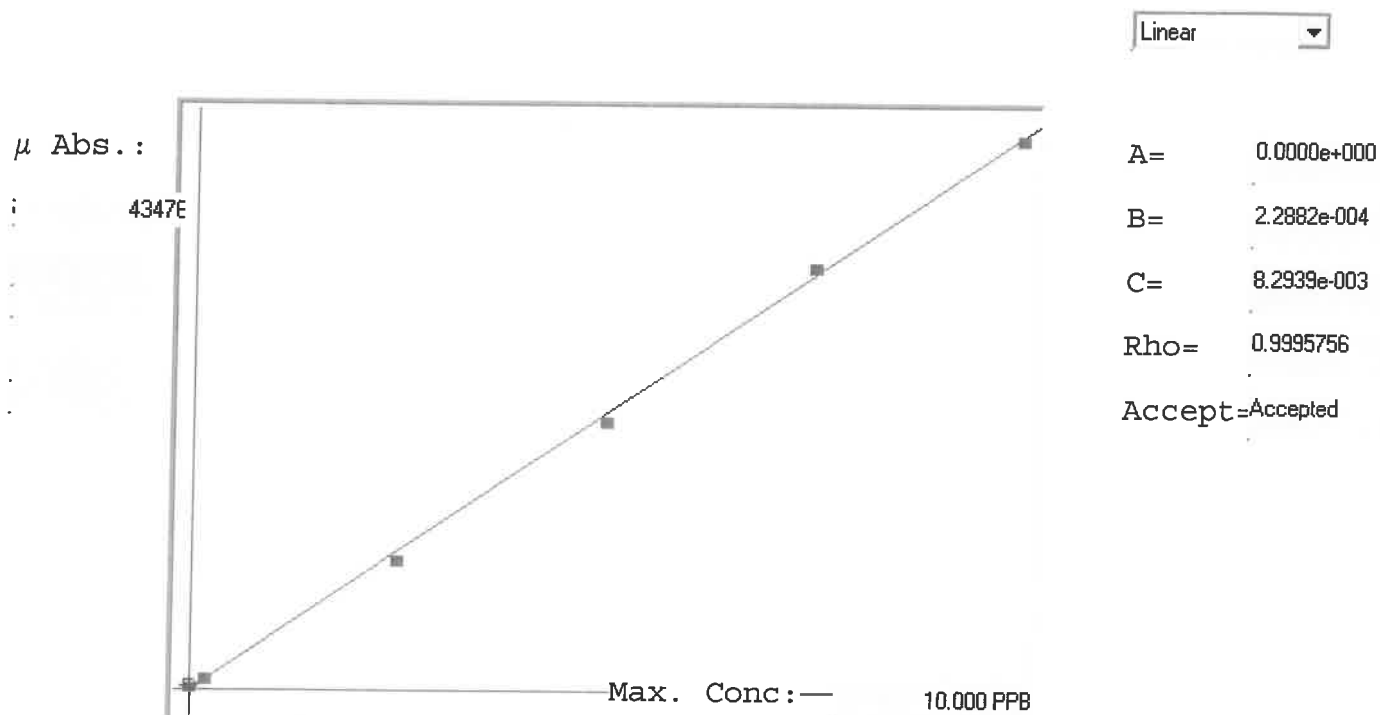

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/6 D
0.0	0.000	0.077	0.077	301	0.000	301	0				
0.2	0.200	0.247	0.047	1045	0.0 %	1045					24
2.5	2.500	2.362	-0.138	10288	0.0 %	10288					-6
5.0	5.000	4.889	-0.111	21332	0.0 %	21332					-2
7.5	7.500	7.667	0.167	33473	0.0 %	33473					2
10.0	10.000	9.956	-0.044	43476	0.0 %	43476					0

LB130313 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 15 Apr 2024 11:49:01

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	301	-	0.0000	7470A	PPB	15 Apr 2024 12:07:07	S	Std
0.2 - 1	50.2	1045	-	0.2000	7470A	PPB	15 Apr 2024 12:09:24	S	Std
2.5 - 1	52.5	10288	-	2.5000	7470A	PPB	15 Apr 2024 12:11:41	S	Std
5.0 - 1	55	21332	-	5.0000	7470A	PPB	15 Apr 2024 12:13:58	S	Std
7.5 - 1	57.5	33473	-	7.5000	7470A	PPB	15 Apr 2024 12:23:59	S	Std
10.0 - 1	540	43476	-	10.0000	7470A	PPB	15 Apr 2024 12:29:00	S	Std
ICV96 - 1	ICV96	16865	3.8673	-	7470A	PPB	15 Apr 2024 12:31:48	U	SMPL
ICB96 - 1	ICB96	249	0.0653	-	7470A	PPB	15 Apr 2024 12:34:04	U	SMPL
CCV16 - 1	CCV16	22103	5.0658	-	7470A	PPB	15 Apr 2024 12:39:01	U	SMPL
CCB16 - 1	CCB16	301	0.0772	-	7470A	PPB	15 Apr 2024 12:41:16	U	SMPL
CRA - 1	CRA	928	0.2206	-	7470A	PPB	15 Apr 2024 12:43:34	U	SMPL
HighStd - 1	HighStd	43214	9.8963	-	7470A	PPB	15 Apr 2024 12:45:49	U	SMPL
ChkStd - 1	ChkStd	30457	6.9773	-	7470A	PPB	15 Apr 2024 12:48:04	U	SMPL
PB160211BL - 1	PBW	-77	-0.0093	-	7470A	PPB	15 Apr 2024 12:50:23	U	SMPL
PB160211BS - 1	LCSW	17914	4.1073	-	7470A	PPB	15 Apr 2024 12:52:41	U	SMPL
P2070-02 - 1	TP-1	24	0.0138	-	7470A	PPB	15 Apr 2024 12:54:57	U	SMPL
P2070-04 - 1	TP-2	446	0.1103	-	7470A	PPB	15 Apr 2024 12:57:16	U	SMPL
P2070-06 - 1	TP-3	369	0.0927	-	7470A	PPB	15 Apr 2024 12:59:34	U	SMPL
P2070-08 - 1	TP-4	427	0.1060	-	7470A	PPB	15 Apr 2024 13:01:51	U	SMPL
P2070-10 - 1	TP-5	389	0.0973	-	7470A	PPB	15 Apr 2024 13:04:07	U	SMPL
CCV17 - 1	CCV17	20831	4.7747	-	7470A	PPB	15 Apr 2024 13:06:23	U	SMPL
CCB17 - 1	CCB17	309	0.0790	-	7470A	PPB	15 Apr 2024 13:08:38	U	SMPL
P2070-10DUP - 1	TP-5DUP	456	0.1126	-	7470A	PPB	15 Apr 2024 13:10:55	U	SMPL
P2070-10MS - 1	TP-5MS	15878	3.6414	-	7470A	PPB	15 Apr 2024 13:13:11	U	SMPL
P2070-10MSD - 1	TP-5MSD	16419	3.7652	-	7470A	PPB	15 Apr 2024 13:15:26	U	SMPL
PB160212BL - 1	PBW	248	0.0650	-	7470A	PPB	15 Apr 2024 13:17:44	U	SMPL
PB160212BS - 1	LCSW	18262	4.1869	-	7470A	PPB	15 Apr 2024 13:20:02	U	SMPL
P2066-01 - 1	T3438	207	0.0557	-	7470A	PPB	15 Apr 2024 13:22:18	U	SMPL
P2066-02 - 1	T3484	373	0.0936	-	7470A	PPB	15 Apr 2024 13:24:37	U	SMPL
P2066-02DUP - 1	T3484DUP	420	0.1044	-	7470A	PPB	15 Apr 2024 13:26:54	U	SMPL
P2066-02MS - 1	T3484MS	16350	3.7494	-	7470A	PPB	15 Apr 2024 13:29:11	U	SMPL
P2066-02MSD - 1	T3484MSD	17052	3.9101	-	7470A	PPB	15 Apr 2024 13:31:27	U	SMPL
CCV18 - 1	CCV18	20687	4.7418	-	7470A	PPB	15 Apr 2024 13:33:45	U	SMPL
CCB18 - 1	CCB18	210	0.0563	-	7470A	PPB	15 Apr 2024 13:36:03	U	SMPL
PB160180TB - 1	PB160180TB	259	0.0676	-	7470A	PPB	15 Apr 2024 13:38:21	U	SMPL
PB160182TB - 1	PB160182TB	319	0.0813	-	7470A	PPB	15 Apr 2024 13:40:36	U	SMPL
P2070-10LX5 - 1		294	0.0756	-	7470A	PPB	15 Apr 2024 13:42:52	U	SMPL
P2070-10A - 1		14829	3.4014	-	7470A	PPB	15 Apr 2024 13:45:08	U	SMPL
P2066-02LX5 - 1		155	0.0438	-	7470A	PPB	15 Apr 2024 13:47:23	U	SMPL
P2066-02A - 1		14797	3.3941	-	7470A	PPB	15 Apr 2024 13:49:42	U	SMPL
CCV19 - 1	CCV19	21335	4.8901	-	7470A	PPB	15 Apr 2024 13:51:59	U	SMPL
CCB19 - 1	CCB19	118	0.0353	-	7470A	PPB	15 Apr 2024 13:54:18	U	SMPL