


LB130324

7471B

INSTRUMENT 1) : CVI

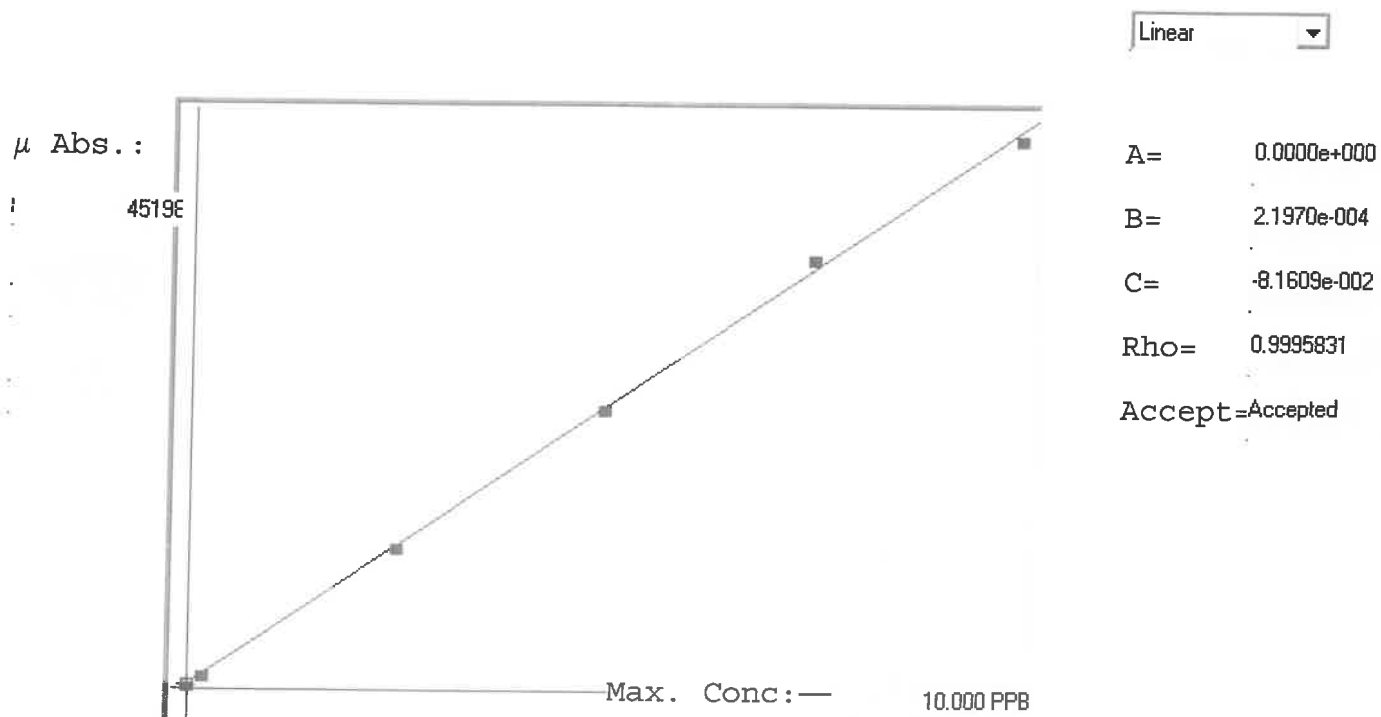

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.015	0.015	439	0.000	439					—
0.2	0.200	0.163	-0.037	1113	0.0 %	1113					-19
2.5	2.500	2.473	-0.027	11627	0.0 %	11627					-1
5.0	5.000	4.994	-0.006	23101	0.0 %	23101					0
7.5	7.500	7.707	0.207	35450	0.0 %	35450					3
10.0	10.000	9.849	-0.151	45198	0.0 %	45198					-2

LB130324 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 16 Apr 2024 09:20:41

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	439	-	0.0000	7471B	PPB	16 Apr 2024 09:50:55	S	Std
0.2 - 1	50.2	1113	-	0.2000	7471B	PPB	16 Apr 2024 09:53:12	S	Std
2.5 - 1	52.5	11627	-	2.5000	7471B	PPB	16 Apr 2024 09:55:30	S	Std
5.0 - 1	55	23101	-	5.0000	7471B	PPB	16 Apr 2024 09:57:47	S	Std
7.5 - 1	57.5	35450	-	7.5000	7471B	PPB	16 Apr 2024 10:02:45	S	Std
10.0 - 1	510	45198	-	10.0000	7471B	PPB	16 Apr 2024 10:07:51	S	Std
ICV97 - 1	ICV97	19687	4.2437	-	7471B	PPB	16 Apr 2024 10:10:42	U	SMPL
ICB97 - 1	ICB97	219	-0.0335	-	7471B	PPB	16 Apr 2024 10:15:41	U	SMPL
CCV19 - 1	CCV19	23881	5.1652	-	7471B	PPB	16 Apr 2024 10:17:56	U	SMPL
CCB19 - 1	CCB19	244	-0.0280	-	7471B	PPB	16 Apr 2024 10:22:51	U	SMPL
CRA - 1	CRA	1087	0.1572	-	7471B	PPB	16 Apr 2024 10:25:06	U	SMPL
HighStd - 1	HighStd	46153	10.0584	-	7471B	PPB	16 Apr 2024 10:27:22	U	SMPL
ChkStd - 1	ChkStd	31999	6.9487	-	7471B	PPB	16 Apr 2024 10:29:39	U	SMPL
PB160281BL - 1	PBS	279	-0.0203	-	7471B	PPB	16 Apr 2024 10:34:50	U	SMPL
PB160281BS - 1	LCSS	19186	4.1336	-	7471B	PPB	16 Apr 2024 10:37:07	U	SMPL
P2108-03 - 1	286	10145	2.1473	-	7471B	PPB	16 Apr 2024 10:39:23	U	SMPL
P2114-01 - 1	NB-08-041224	2598	0.4892	-	7471B	PPB	16 Apr 2024 10:41:44	U	SMPL
P2114-01DUP - 1	NB-08-041224DUP	2749	0.5224	-	7471B	PPB	16 Apr 2024 10:59:06	U	SMPL
P2114-01MS - 1	NB-08-041224MS	21376	4.6148	-	7471B	PPB	16 Apr 2024 11:04:06	U	SMPL
P2114-01MSD - 1	NB-08-041224MSD	21523	4.6471	-	7471B	PPB	16 Apr 2024 11:06:22	U	SMPL
CCV20 - 1	CCV20	21738	4.6943	-	7471B	PPB	16 Apr 2024 11:18:03	U	SMPL
CCB20 - 1	CCB20	28	-0.0755	-	7471B	PPB	16 Apr 2024 11:20:18	U	SMPL
P2126-01 - 1	SP-1A	32552	7.0702	-	7471B	PPB	16 Apr 2024 11:22:37	U	SMPL
P2126-04 - 1	SP-1B	25680	5.5604	-	7471B	PPB	16 Apr 2024 11:24:53	U	SMPL
P2126-07 - 1	SP-1C	13404	2.8633	-	7471B	PPB	16 Apr 2024 11:27:11	U	SMPL
P2127-01 - 1	SP-2-FRONT	84227	18.4235	-	7471B	PPB	16 Apr 2024 11:29:31	U	SMPL
P2127-04 - 1	SP-2-BACK	23923	5.1744	-	7471B	PPB	16 Apr 2024 11:31:51	U	SMPL
P2114-01LX5 - 1		234	-0.0302	-	7471B	PPB	16 Apr 2024 11:40:34	U	SMPL
P2114-01A - 1		21117	4.5579	-	7471B	PPB	16 Apr 2024 11:42:50	U	SMPL
P2127-01DLX5 - 1		18973	4.0869	-	7471B	PPB	16 Apr 2024 11:45:07	U	SMPL
CCV21 - 1	CCV21	24608	5.3249	-	7471B	PPB	16 Apr 2024 11:47:30	U	SMPL
CCB21 - 1	CCB21	260	-0.0245	-	7471B	PPB	16 Apr 2024 11:49:51	U	SMPL