

16130353

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

4/17/2024 10:43

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	94.221	0.0	0.089	
ICB001 ICB001	1.711	0.0	0.003	
CCV001 CCV001	242.646	0.0	0.227	
CCB001 CCB001	1.255	0.0	0.002	
PB160323BL PBS323	0.891	0.0	0.002	
P2146-01 E07W9	0.346	0.0	0.001	
P2146-03 E07X1	0.809	0.0	0.002	
P2146-04 E07X2	0.644	0.0	0.002	
P2146-05 E07X3	2.919	0.0	0.004	
P2146-06 E07Y0	0.610	0.0	0.002	
P2146-07 E07Y1	-0.502	0.0	0.001	
P2146-08 E07Y2	0.037	0.0	0.001	
P2146-09 E07Y3	0.295	0.0	0.001	
P2146-10 E07Y4	-0.197	0.0	0.001	
P2146-11 E07Y4D	-0.630	0.0	0.000	
P2146-12 E07Y4S	93.606	0.0	0.088	
P2146-13 E07Y5	0.866	0.0	0.002	
P2146-02 E07X0	1.301	0.0	0.002	
PB160324BL PBW324	1.187	0.0	0.002	
P2146-15 E07Z8	-0.291	0.0	0.001	
CCV002 CCV002	248.092	0.0	0.232	
CCB002 CCB002	0.836	0.0	0.002	

N	22
Mean	31.393
SD	74.4521
CV%	237.16

04/17/2024
RM04/17/24
RM

Aquakem v. 7.2AQ1

Results from time period:

Wed Apr 17 08:43:34 2024

Wed Apr 17 10:39:08 2024

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NEW	P	1.0842	µg/l	4/17/2024 9:00:36
S5.0	A	CNEPA-NEW	P	4.2123	µg/l	4/17/2024 9:00:37
S10.0	A	CNEPA-NEW	P	9.1646	µg/l	4/17/2024 9:00:38
S100.0	A	CNEPA-NEW	P	98.3489	µg/l	4/17/2024 9:00:39
S250.0	A	CNEPA-NEW	P	253.6703	µg/l	4/17/2024 9:00:40
S500.0	A	CNEPA-NEW	P	498.5196	µg/l	4/17/2024 9:00:41
ICV001 ICV001	S	CNEPA-NEW	P	94.2213	µg/l	4/17/2024 10:01:34
ICB001 ICB001	S	CNEPA-NEW	P	1.7108	µg/l	4/17/2024 10:01:36
CCV001 CCV001	S	CNEPA-NEW	P	242.6464	µg/l	4/17/2024 10:01:38
CCB001 CCB001	S	CNEPA-NEW	P	1.2555	µg/l	4/17/2024 10:01:40
PB160323BL PBS323	S	CNEPA-NEW	P	0.8909	µg/l	4/17/2024 10:01:41
P2146-01 E07W9	S	CNEPA-NEW	P	0.3464	µg/l	4/17/2024 10:01:43
P2146-03 E07X1	S	CNEPA-NEW	P	0.8088	µg/l	4/17/2024 10:09:09
P2146-04 E07X2	S	CNEPA-NEW	P	0.6439	µg/l	4/17/2024 10:09:10
P2146-05 E07X3	S	CNEPA-NEW	P	2.9193	µg/l	4/17/2024 10:09:11
P2146-06 E07Y0	S	CNEPA-NEW	P	0.6097	µg/l	4/17/2024 10:09:12
P2146-07 E07Y1	S	CNEPA-NEW	P	-0.5025	µg/l	4/17/2024 10:09:13
P2146-08 E07Y2	S	CNEPA-NEW	P	0.0372	µg/l	4/17/2024 10:09:14
P2146-09 E07Y3	S	CNEPA-NEW	P	0.2954	µg/l	4/17/2024 10:09:15
P2146-10 E07Y4	S	CNEPA-NEW	P	-0.197	µg/l	4/17/2024 10:09:16
P2146-11 E07Y4D	S	CNEPA-NEW	P	-0.6297	µg/l	4/17/2024 10:09:18
P2146-12 E07Y4S	S	CNEPA-NEW	P	93.6063	µg/l	4/17/2024 10:16:44
P2146-13 E07Y5	S	CNEPA-NEW	P	0.866	µg/l	4/17/2024 10:16:45
P2146-02 E07X0	S	CNEPA-NEW	P	1.3008	µg/l	4/17/2024 10:16:46
PB160324BL PBW324	S	CNEPA-NEW	P	1.1867	µg/l	4/17/2024 10:16:48
P2146-15 E07Z8	S	CNEPA-NEW	P	-0.2909	µg/l	4/17/2024 10:16:50
CCV002 CCV002	S	CNEPA-NEW	P	248.0917	µg/l	4/17/2024 10:22:27
CCB002 CCB002	S	CNEPA-NEW	P	0.836	µg/l	4/17/2024 10:22:30

CHEMTECH CONSULTING GROUP INC
 284 Sheffield Street, Mountainside, NJ 07092

4/17/2024 9:13 Reviewed by : RM Instrument ID : Konelab


Test CNEPA-NEW

Accepted 4/17/2024 9:13

Factor slope 1072 0.000933
 Bias y intercept 0.001 04/18/2024
 RM

Coeff. of det. 0.999894

Errors

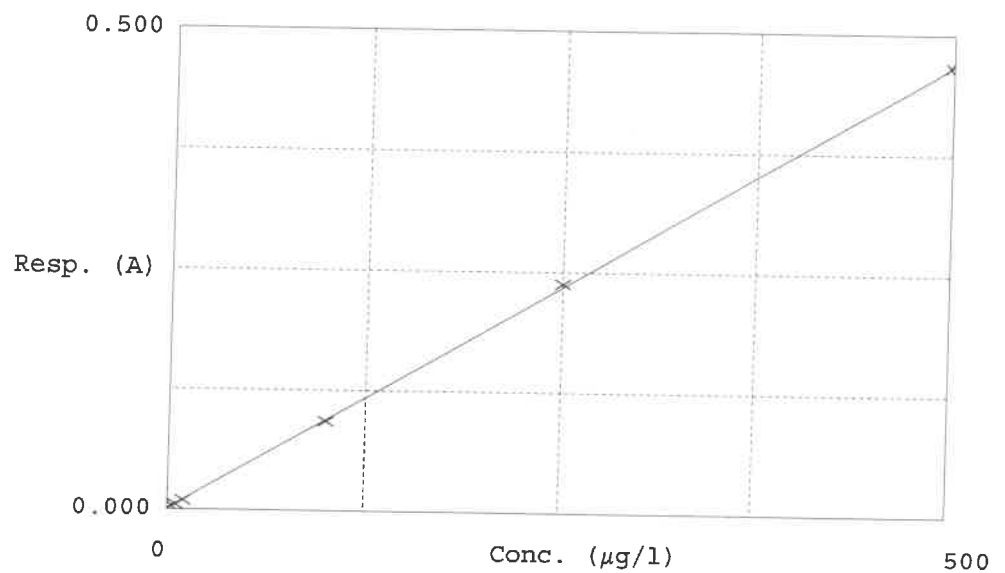

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN\$0.0	0.002	1.0842	0.0000	-
2	5.0PPBCN\$5.0	0.005	4.2123	5.0000	-15.8
3	10PPBCN \$10.0	0.010	9.1646	10.0000	-8.4
4	100PPBCN\$100.0	0.093	98.3489	100.0000	-1.7
5	250PPBCN \$250.0	0.238	253.6703	250.0000	1.5
6	500PPBCN\$500.0	0.466	498.5196	500.0000	-0.3

04/17/2024
 RM