


7470A

INSTRUMENT ID: CV 1

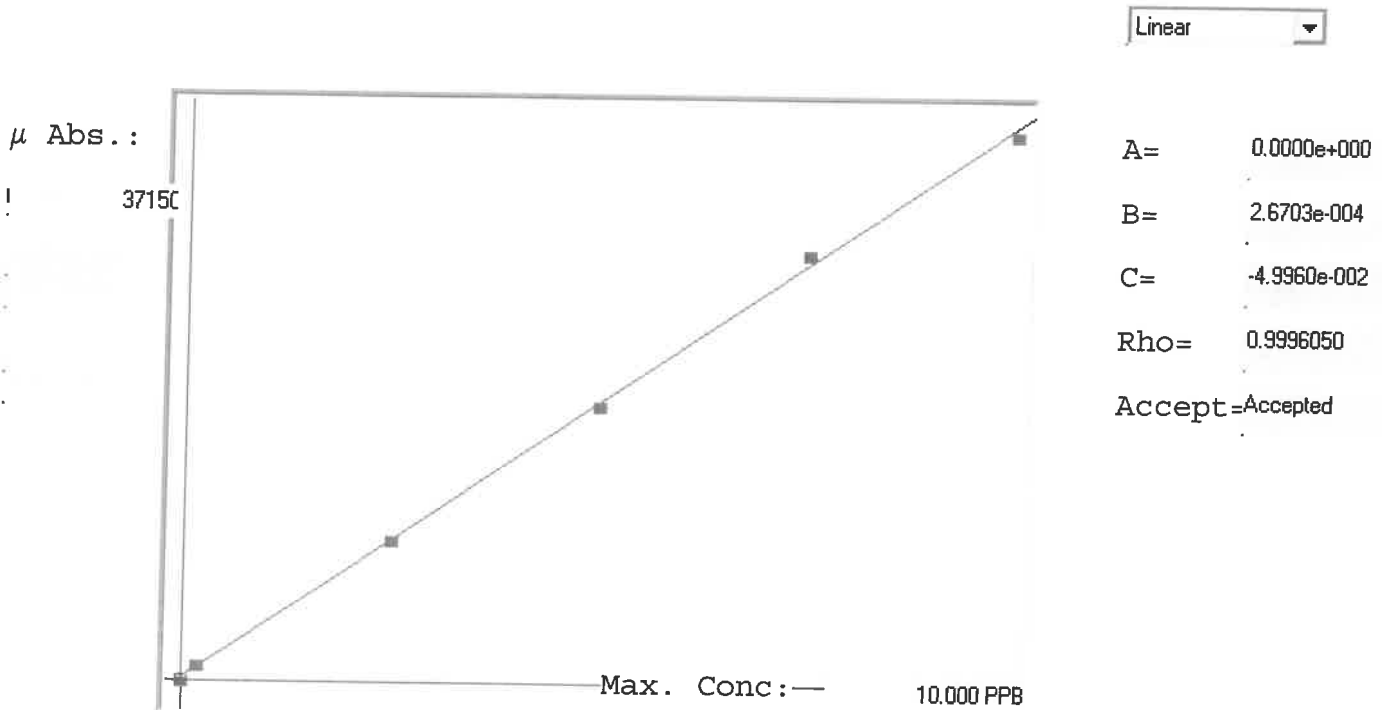

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.074	-0.074	-91	0.000	-91	0			
0.2	0.200	0.256	0.056	1144	0.0 %	1144				
2.5	2.500	2.501	0.001	9552	0.0 %	9552				
5.0	5.000	4.955	-0.045	18744	0.0 %	18744				
7.5	7.500	7.693	0.193	28995	0.0 %	28995				
10.0	10.000	9.870	-0.130	37150	0.0 %	37150				

LB130377 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 18 Apr 2024 12:05:22

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	370	-91	-	0.0000	7470A	PPB	18 Apr 2024 12:14:41	S	Std
0.2 - 1	50.2	1144	-	0.2000	7470A	PPB	18 Apr 2024 12:16:58	S	Std
2.5 - 1	32.5	9552	-	2.5000	7470A	PPB	18 Apr 2024 12:19:15	S	Std
5.0 - 1	95	18744	-	5.0000	7470A	PPB	18 Apr 2024 12:21:32	S	Std
7.5 - 1	57.5	28995	-	7.5000	7470A	PPB	18 Apr 2024 12:23:51	S	Std
10.0 - 1	57.4	37150	-	10.0000	7470A	PPB	18 Apr 2024 12:31:48	S	Std
ICV02 - 1	ICV02	16079	4.2436	-7470A	PPB	18 Apr 2024 12:34:50	U	SMPL	
ICB02 - 1	ICB02	72	-0.0307	-7470A	PPB	18 Apr 2024 12:39:41	U	SMPL	
CCV31 - 1	CCV31	20327	5.3780	-7470A	PPB	18 Apr 2024 12:41:56	U	SMPL	
CCB31 - 1	CCB31	-90	-0.0740	-7470A	PPB	18 Apr 2024 12:46:49	U	SMPL	
CRA - 1	CRA	913	0.1938	-7470A	PPB	18 Apr 2024 12:49:04	U	SMPL	
HighStd - 1	HighStd	38308	10.1794	-7470A	PPB	18 Apr 2024 12:51:18	U	SMPL	
ChkStd - 1	ChkStd	29439	7.8111	-7470A	PPB	18 Apr 2024 12:53:34	U	SMPL	
PB160318BL - 1	PBW	-147	-0.0892	-7470A	PPB	18 Apr 2024 12:58:30	U	SMPL	
PB160318BS - 1	LCSW	14328	3.7760	-7470A	PPB	18 Apr 2024 13:03:23	U	SMPL	
P2122-01 - 1	M-R-OILY-DEBRIS	-95	-0.0753	-7470A	PPB	18 Apr 2024 13:05:40	U	SMPL	
P2126-02 - 1	SP-1A	76	-0.0297	-7470A	PPB	18 Apr 2024 13:07:58	U	SMPL	
P2126-05 - 1	SP-1B	237	0.0133	-7470A	PPB	18 Apr 2024 13:10:16	U	SMPL	
P2126-08 - 1	SP-1C	466	0.0745	-7470A	PPB	18 Apr 2024 13:12:33	U	SMPL	
P2127-02 - 1	SP-2-FRONT	285	0.0261	-7470A	PPB	18 Apr 2024 13:14:49	U	SMPL	
CCV32 - 1	CCV32	18289	4.8338	-7470A	PPB	18 Apr 2024 13:19:40	U	SMPL	
CCB32 - 1	CCB32	-21	-0.0556	-7470A	PPB	18 Apr 2024 13:24:39	U	SMPL	
P2127-05 - 1	SP-2-BACK	224	0.0099	-7470A	PPB	18 Apr 2024 13:26:54	U	SMPL	
P2127-05DUP - 1	SP-2-BACKDUP	316	0.0344	-7470A	PPB	18 Apr 2024 13:29:10	U	SMPL	
P2127-05MS - 1	SP-2-BACKMS	15944	4.2076	-7470A	PPB	18 Apr 2024 13:34:09	U	SMPL	
P2127-05MSD - 1	SP-2-BACKMSD	13745	3.6204	-7470A	PPB	18 Apr 2024 13:36:24	U	SMPL	
PB160319BL - 1	PBW	174	-0.0035	-7470A	PPB	18 Apr 2024 13:41:24	U	SMPL	
PB160319BS - 1	LCSW	17220	4.5483	-7470A	PPB	18 Apr 2024 13:43:40	U	SMPL	
P2108-02 - 1	T3505	-152	-0.0905	-7470A	PPB	18 Apr 2024 13:45:57	U	SMPL	
P2108-02DUP - 1	T3505DUP	254	0.0179	-7470A	PPB	18 Apr 2024 13:48:17	U	SMPL	
P2108-02MS - 1	T3505MS	15634	4.1248	-7470A	PPB	18 Apr 2024 13:53:13	U	SMPL	
P2108-02MSD - 1	T3505MSD	15972	4.2150	-7470A	PPB	18 Apr 2024 13:55:30	U	SMPL	
CCV33 - 1	CCV33	18545	4.9021	-7470A	PPB	18 Apr 2024 13:57:48	U	SMPL	
CCB33 - 1	CCB33	-176	-0.0970	-7470A	PPB	18 Apr 2024 14:00:06	U	SMPL	
PB160258TB - 1	PB160258TB	196	0.0024	-7470A	PPB	18 Apr 2024 14:02:25	U	SMPL	
PB160259TB - 1	PB160259TB	254	0.0179	-7470A	PPB	18 Apr 2024 14:04:40	U	SMPL	
P2127-05LX5 - 1		-88	-0.0735	-7470A	PPB	18 Apr 2024 14:06:56	U	SMPL	
P2127-05A - 1		16976	4.4831	-7470A	PPB	18 Apr 2024 14:09:12	U	SMPL	
P2108-02LX5 - 1		-446	-0.1691	-7470A	PPB	18 Apr 2024 14:11:28	U	SMPL	
P2108-02A - 1		17581	4.6447	-7470A	PPB	18 Apr 2024 14:13:48	U	SMPL	
CCV34 - 1	CCV34	19959	5.2797	-7470A	PPB	18 Apr 2024 14:24:31	U	SMPL	
CCB34 - 1	CCB34	-75	-0.0700	-7470A	PPB	18 Apr 2024 14:26:48	U	SMPL	