


LB180491

7471B

INSTRUMENT ID: CV1

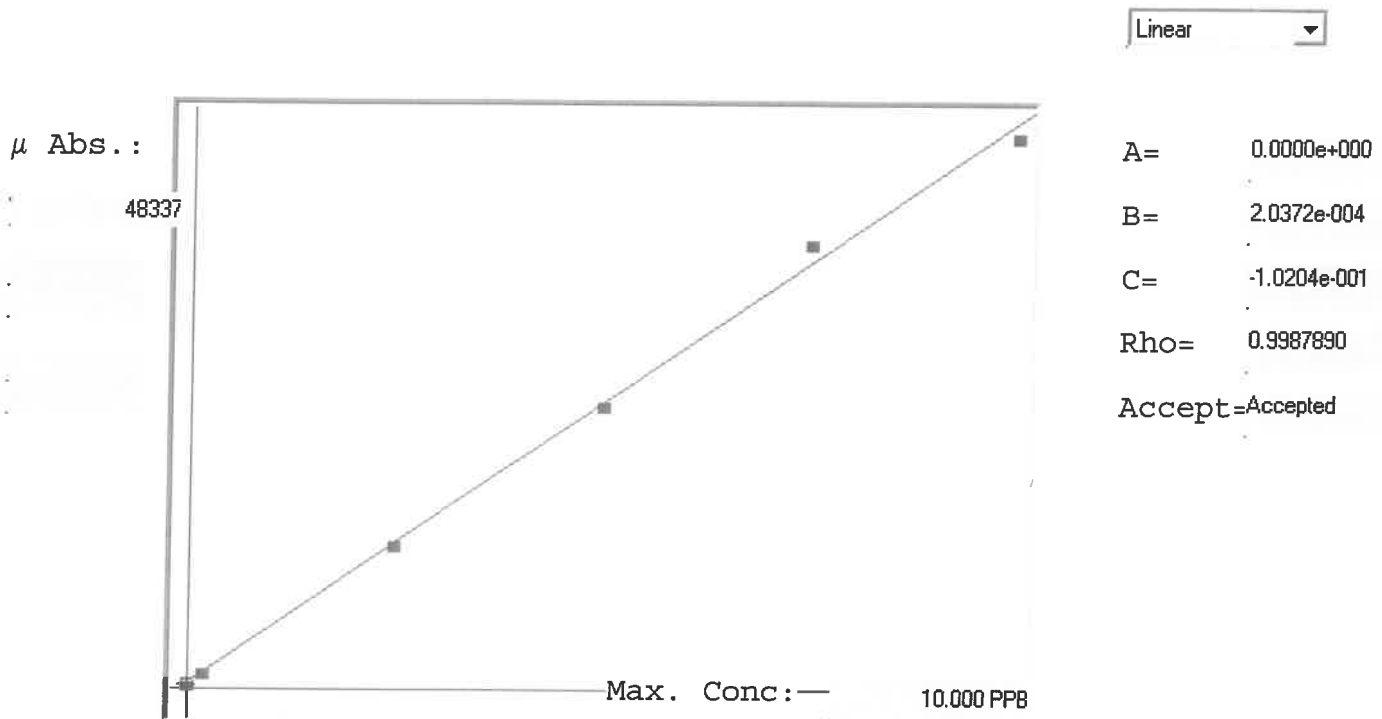

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.0	0.000	-0.018	-0.018	413	0.000	413					
0.2	0.200	0.193	-0.007	1450	0.0 %	1450					-4
2.5	2.500	2.477	-0.023	12661	0.0 %	12661					-1
5.0	5.000	4.943	-0.057	24764	0.0 %	24764					-1
7.5	7.500	7.859	0.359	39077	0.0 %	39077					5
10.0	10.000	9.745	-0.255	48337	0.0 %	48337					-3

LB130491 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 25 Apr 2024 13:30:59

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	413	-	0.000	7471B	PPB	25 Apr 2024 14:08:02	S	Std
0.2 - 1	50.2	1450	-	0.200	7471B	PPB	25 Apr 2024 14:10:19	S	Std
2.5 - 1	52.5	12661	-	2.500	7471B	PPB	25 Apr 2024 14:12:36	S	Std
5.0 - 1	55	24764	-	5.000	7471B	PPB	25 Apr 2024 14:14:53	S	Std
7.5 - 1	57.5	39077	-	7.500	7471B	PPB	25 Apr 2024 14:17:13	S	Std
10.0 - 1	57.6	48337	-	10.000	7471B	PPB	25 Apr 2024 14:22:42	S	Std
ICV14 - 1	ICV14	19141	3.7974	-	7471B	PPB	25 Apr 2024 14:28:14	U	SMPL
ICB14 - 1	ICB14	169	-0.0676	-	7471B	PPB	25 Apr 2024 14:30:28	U	SMPL
CCV72 - 1	CCV72	24454	4.8798	-	7471B	PPB	25 Apr 2024 14:32:49	U	SMPL
CCB72 - 1	CCB72	42	-0.0935	-	7471B	PPB	25 Apr 2024 14:35:04	U	SMPL
CRA - 1	CRA	1329	0.1687	-	7471B	PPB	25 Apr 2024 14:37:27	U	SMPL
HighStd - 1	HighStd	46678	9.4074	-	7471B	PPB	25 Apr 2024 14:39:42	U	SMPL
ChkStd - 1	ChkStd	34455	6.9173	-	7471B	PPB	25 Apr 2024 14:41:59	U	SMPL
PB160525BL - 1	PBS	51	-0.0917	-	7471B	PPB	25 Apr 2024 14:44:26	U	SMPL
PB160525BS - 1	LCSS	18845	3.7371	-	7471B	PPB	25 Apr 2024 14:46:54	U	SMPL
P2240-02 - 1	AU-05-042324	14512	2.8544	-	7471B	PPB	25 Apr 2024 14:49:11	U	SMPL
P2241-01 - 1	344	425	-0.0155	-	7471B	PPB	25 Apr 2024 14:51:32	U	SMPL
P2245-01 - 1	YARD-3	581	0.0163	-	7471B	PPB	25 Apr 2024 14:53:54	U	SMPL
P2247-01 - 1	PL-02-04232024	1529	0.2095	-	7471B	PPB	25 Apr 2024 14:56:11	U	SMPL
P2247-04 - 1	PL-03-04232024	2581	0.4238	-	7471B	PPB	25 Apr 2024 14:58:27	U	SMPL
CCV73 - 1	CCV73	24058	4.7992	-	7471B	PPB	25 Apr 2024 15:00:44	U	SMPL
CCB73 - 1	CCB73	41	-0.0937	-	7471B	PPB	25 Apr 2024 15:03:00	U	SMPL
P2257-02 - 1	1356	375	-0.0256	-	7471B	PPB	25 Apr 2024 15:05:22	U	SMPL
P2258-01 - 1	OR-03-042424	2742	0.4566	-	7471B	PPB	25 Apr 2024 15:07:37	U	SMPL
P2259-01 - 1	CONCRETE-1	516	0.0031	-	7471B	PPB	25 Apr 2024 15:09:52	U	SMPL
P2259-02 - 1	CONCRETE-2	816	0.0642	-	7471B	PPB	25 Apr 2024 15:12:10	U	SMPL
P2261-01 - 1	RO-RBR200059	2334	0.3734	-	7471B	PPB	25 Apr 2024 15:14:26	U	SMPL
P2262-01 - 1	HR-03-04242024	2237	0.3537	-	7471B	PPB	25 Apr 2024 15:16:43	U	SMPL
P2262-03 - 1	HR-04-04242024	1113	0.1247	-	7471B	PPB	25 Apr 2024 15:25:05	U	SMPL
P2262-03DUP - 1	HR-04-04242024DUP	901	0.0815	-	7471B	PPB	25 Apr 2024 15:34:02	U	SMPL
P2262-03MS - 1	HR-04-04242024MS	23108	4.6056	-	7471B	PPB	25 Apr 2024 15:36:19	U	SMPL
P2262-03MSD - 1	HR-04-04242024MSD	22622	4.5066	-	7471B	PPB	25 Apr 2024 15:38:35	U	SMPL
CCV74 - 1	CCV74	27439	5.4879	-	7471B	PPB	25 Apr 2024 15:40:55	U	SMPL
CCB74 - 1	CCB74	117	-0.0782	-	7471B	PPB	25 Apr 2024 15:43:16	U	SMPL
P2262-01LX5 - 1		271	-0.0468	-	7471B	PPB	25 Apr 2024 15:45:38	U	SMPL
P2262-01A - 1		20441	4.0623	-	7471B	PPB	25 Apr 2024 15:47:53	U	SMPL
CCV75 - 1	CCV75	26134	5.2221	-	7471B	PPB	25 Apr 2024 15:50:09	U	SMPL
CCB75 - 1	CCB75	321	-0.0366	-	7471B	PPB	25 Apr 2024 15:56:57	U	SMPL