


LB130555

7471B

INSTRUMENT ID: CV2

Linear

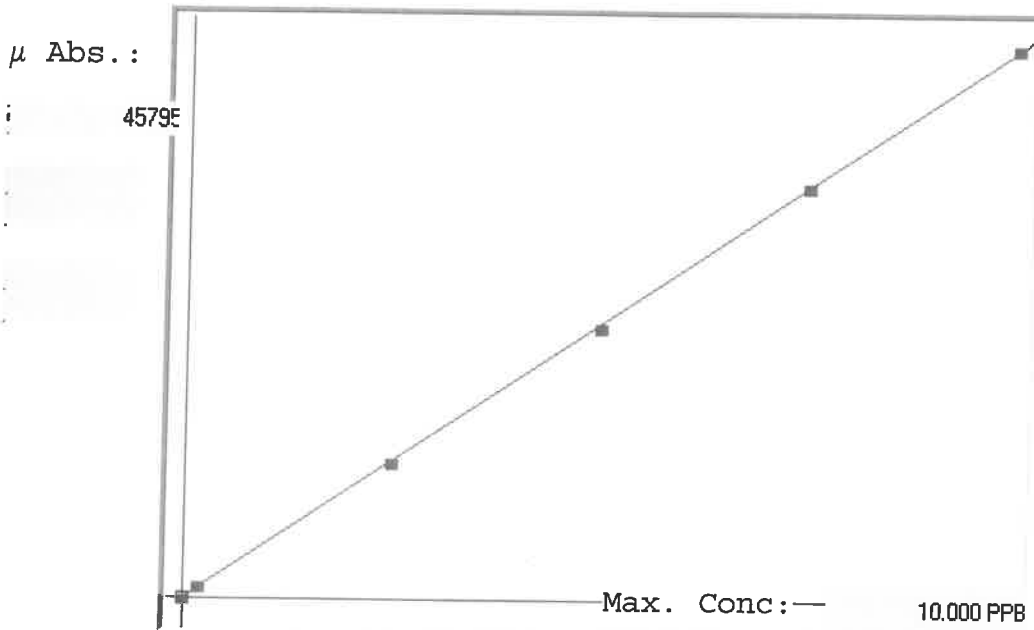

A= 0.0000e+000

B= 2.1902e-004

C= -4.1011e-003

Rho= 0.9999767

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%
0.0	0.000	0.027	0.027	140	0.000	140					
0.2	0.200	0.208	0.008	967	0.0 %	967					
2.5	2.500	2.486	-0.014	11369	0.0 %	11369					
5.0	5.000	4.953	-0.047	22635	0.0 %	22635					
7.5	7.500	7.500	0.000	34263	0.0 %	34263					
10.0	10.000	10.026	0.026	45795	0.0 %	45795					

4/00

14

11

11

00

LB130555 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 30 Apr 2024 10:11:58

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	140	-	0.0000	7471B	PPB	30 Apr 2024 10:26:40	S	Std
0.2 - 1	50.2	967	-	0.2000	7471B	PPB	30 Apr 2024 10:28:57	S	Std
2.5 - 1	52.5	11369	-	2.5000	7471B	PPB	30 Apr 2024 10:34:34	S	Std
5.0 - 1	55	22635	-	5.0000	7471B	PPB	30 Apr 2024 10:36:51	S	Std
7.5 - 1	57.5	34263	-	7.5000	7471B	PPB	30 Apr 2024 10:39:10	S	Std
10.0 - 1	510	45795	-	10.0000	7471B	PPB	30 Apr 2024 10:44:16	S	Std
ICV20 - 1	ICV20	19153	4.1908	-	7471B	PPB	30 Apr 2024 10:52:43	U	SMPL
ICB20 - 1	ICB20	-240	-0.0567	-	7471B	PPB	30 Apr 2024 10:55:00	U	SMPL
CCV90 - 1	CCV90	25081	5.4892	-	7471B	PPB	30 Apr 2024 10:57:18	U	SMPL
CCB90 - 1	CCB90	-253	-0.0595	-	7471B	PPB	30 Apr 2024 10:59:33	U	SMPL
CRA - 1	CRA	1026	0.2206	-	7471B	PPB	30 Apr 2024 11:01:54	U	SMPL
HighStd - 1	HighStd	48324	10.5799	-	7471B	PPB	30 Apr 2024 11:04:09	U	SMPL
ChkStd - 1	ChkStd	34591	7.5721	-	7471B	PPB	30 Apr 2024 11:06:25	U	SMPL
PB160616BL - 1	PBS	-434	-0.0992	-	7471B	PPB	30 Apr 2024 11:08:51	U	SMPL
PB160616BS - 1	LCSS	16959	3.7103	-	7471B	PPB	30 Apr 2024 11:11:16	U	SMPL
P2270-01 - 1	72-11936	3280	0.7143	-	7471B	PPB	30 Apr 2024 11:22:57	U	SMPL
P2270-01DUP - 1	72-11936DUP	3146	0.6849	-	7471B	PPB	30 Apr 2024 11:25:14	U	SMPL
P2270-01MS - 1	72-11936MS	24843	5.4371	-	7471B	PPB	30 Apr 2024 11:27:33	U	SMPL
P2270-01MSD - 1	72-11936MSD	23104	5.0562	-	7471B	PPB	30 Apr 2024 11:29:51	U	SMPL
P2270-03 - 1	VNJ-240	5421	1.1832	-	7471B	PPB	30 Apr 2024 11:32:10	U	SMPL
CCV91 - 1	CCV91	21984	4.8109	-	7471B	PPB	30 Apr 2024 11:38:08	U	SMPL
CCB91 - 1	CCB91	-98	-0.0256	-	7471B	PPB	30 Apr 2024 11:40:23	U	SMPL
P2271-01 - 1	RT-3860	2104	0.4567	-	7471B	PPB	30 Apr 2024 11:42:43	U	SMPL
P2274-02 - 1	VNJ-209	4884	1.0656	-	7471B	PPB	30 Apr 2024 11:44:58	U	SMPL
P2274-04 - 1	DRUMP-COMP	6213	1.3567	-	7471B	PPB	30 Apr 2024 11:47:15	U	SMPL
P2283-01 - 1	EXCAV-SOIL-1	3489	0.7601	-	7471B	PPB	30 Apr 2024 11:49:32	U	SMPL
P2283-03 - 1	EXCAV-SOIL-2	2816	0.6127	-	7471B	PPB	30 Apr 2024 11:51:50	U	SMPL
P2294-01 - 1	FOOT-PRINT-A-1	4533	0.9887	-	7471B	PPB	30 Apr 2024 11:54:08	U	SMPL
P2294-02 - 1	FOOT-PRINT-A-2	13255	2.8990	-	7471B	PPB	30 Apr 2024 11:56:25	U	SMPL
P2294-03 - 1	FOOT-PRINT-A-3	3710	0.8085	-	7471B	PPB	30 Apr 2024 11:58:44	U	SMPL
P2294-04 - 1	FOOT-PRINT-B-1	4706	1.0266	-	7471B	PPB	30 Apr 2024 12:01:03	U	SMPL
P2294-05 - 1	FOOT-PRINT-B-2	3532	0.7695	-	7471B	PPB	30 Apr 2024 12:03:20	U	SMPL
CCV92 - 1	CCV92	22815	4.9929	-	7471B	PPB	30 Apr 2024 12:09:49	U	SMPL
CCB92 - 1	CCB92	-40	-0.0129	-	7471B	PPB	30 Apr 2024 12:12:04	U	SMPL
P2294-06 - 1	FOOT-PRINT-B-3	3830	0.8348	-	7471B	PPB	30 Apr 2024 12:14:23	U	SMPL
P2309-01 - 1	TR-05-042924	4148	0.9044	-	7471B	PPB	30 Apr 2024 12:16:38	U	SMPL
P2310-01 - 1	SU-02-042924	4426	0.9653	-	7471B	PPB	30 Apr 2024 12:18:56	U	SMPL
P2310-03 - 1	SU-03-042924	2101	0.4561	-	7471B	PPB	30 Apr 2024 12:21:13	U	SMPL
P2270-01LX5 - 1		469	0.0986	-	7471B	PPB	30 Apr 2024 12:23:31	U	SMPL
P2270-01A - 1		24016	5.2559	-	7471B	PPB	30 Apr 2024 12:25:48	U	SMPL
CCV93 - 1	CCV93	23031	5.0402	-	7471B	PPB	30 Apr 2024 12:30:51	U	SMPL
CCB93 - 1	CCB93	23	0.0009	-	7471B	PPB	30 Apr 2024 12:33:08	U	SMPL