


LB130596

7471B

INSTRUMENT ID: CV1

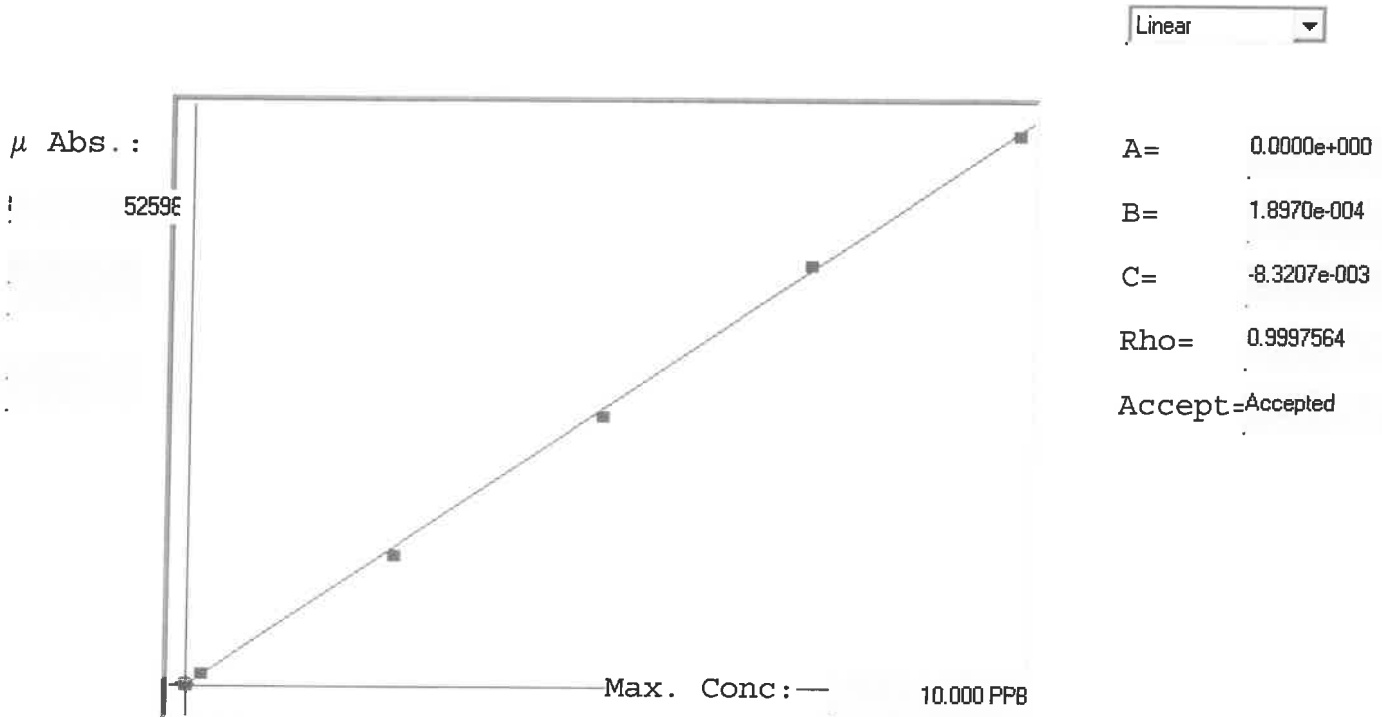

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/01)
0.0	0.000	0.055	0.055	334	0.000	334					
0.2	0.200	0.236	0.036	1290	0.0 %	1290					18
2.5	2.500	2.404	-0.096	12716	0.0 %	12716					4
5.0	5.000	4.906	-0.094	25907	0.0 %	25907					2
7.5	7.500	7.629	0.129	40257	0.0 %	40257					2
10.0	10.000	9.970	-0.030	52598	0.0 %	52598					0

LB130596 INSTRUMENT ID :CV1

Method: 7471B

Operator: Admin

Date of Analysis: 02 May 2024 12:26:17

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	334	-	0.0000	7471B	PPB	02 May 2024 12:36:50	S	Std
0.2 - 1	51.2	1290	-	0.2000	7471B	PPB	02 May 2024 12:39:07	S	Std
2.5 - 1	52.5	12716	-	2.5000	7471B	PPB	02 May 2024 12:41:24	S	Std
5.0 - 1	53	25907	-	5.0000	7471B	PPB	02 May 2024 12:43:42	S	Std
7.5 - 1	54.5	40257	-	7.5000	7471B	PPB	02 May 2024 12:46:01	S	Std
10.0 - 1	518	52598	-	10.0000	7471B	PPB	02 May 2024 12:48:21	S	Std
ICV26 - 1	ICV26	21856	4.1378	-	7471B	PPB	02 May 2024 12:51:21	U	SMPL
ICB26 - 1	ICB26	106	0.0118	-	7471B	PPB	02 May 2024 12:53:38	U	SMPL
CCV07 - 1	CCV07	27720	5.2503	-	7471B	PPB	02 May 2024 12:55:58	U	SMPL
CCB07 - 1	CCB07	-6	-0.0095	-	7471B	PPB	02 May 2024 12:58:13	U	SMPL
CRA - 1	CRA	1172	0.2140	-	7471B	PPB	02 May 2024 13:03:08	U	SMPL
HighStd - 1	HighStd	54110	10.2565	-	7471B	PPB	02 May 2024 13:05:23	U	SMPL
ChkStd - 1	ChkStd	35985	6.8182	-	7471B	PPB	02 May 2024 13:07:38	U	SMPL
PB160668BL - 1	PB160668BL	204	0.0304	-	7471B	PPB	02 May 2024 13:12:41	U	SMPL
PB160668BS - 1	PB160668BS	20760	3.9299	-	7471B	PPB	02 May 2024 13:17:36	U	SMPL
P2307-02 - 1	WC-1	19133	3.6213	-	7471B	PPB	02 May 2024 13:19:53	U	SMPL
P2307-05 - 1	WC-2	4774	0.8973	-	7471B	PPB	02 May 2024 13:22:12	U	SMPL
P2307-08 - 1	WC-3	8347	1.5751	-	7471B	PPB	02 May 2024 13:24:33	U	SMPL
P2322-01 - 1	DEMAREST-MS	1283	0.2351	-	7471B	PPB	02 May 2024 13:26:52	U	SMPL
P2323-01 - 1	TP-1	1341	0.2461	-	7471B	PPB	02 May 2024 13:29:09	U	SMPL
CCV08 - 1	CCV08	27276	5.1660	-	7471B	PPB	02 May 2024 13:31:25	U	SMPL
CCB08 - 1	CCB08	38	-0.0011	-	7471B	PPB	02 May 2024 13:33:40	U	SMPL
P2323-04 - 1	TP-2	2549	0.4752	-	7471B	PPB	02 May 2024 13:35:59	U	SMPL
P2323-07 - 1	TP-3	1156	0.2110	-	7471B	PPB	02 May 2024 13:38:14	U	SMPL
P2326-01 - 1	OK-02-043024	2078	0.3859	-	7471B	PPB	02 May 2024 13:40:31	U	SMPL
P2337-01 - 1	DRT-5204	11567	2.1860	-	7471B	PPB	02 May 2024 13:42:46	U	SMPL
P2337-03 - 1	RB21155-SOIL	4288	0.8051	-	7471B	PPB	02 May 2024 13:45:02	U	SMPL
P2340-01 - 1	VNJ-207	3428	0.6420	-	7471B	PPB	02 May 2024 13:52:26	U	SMPL
P2340-01DUP - 1	VNJ-207DUP	3542	0.6636	-	7471B	PPB	02 May 2024 13:54:44	U	SMPL
P2340-01MS - 1	VNJ-207MS	18265	3.4566	-	7471B	PPB	02 May 2024 13:57:03	U	SMPL
P2340-01MSD - 1	VNJ-207MSD	16966	3.2102	-	7471B	PPB	02 May 2024 13:59:22	U	SMPL
PB160669BL - 1	PB160669BL	133	0.0169	-	7471B	PPB	02 May 2024 14:01:41	U	SMPL
CCV09 - 1	CCV09	28734	5.4426	-	7471B	PPB	02 May 2024 14:03:59	U	SMPL
CCB09 - 1	CCB09	97	0.0101	-	7471B	PPB	02 May 2024 14:06:14	U	SMPL
PB160669BS - 1	PB160669BS	21336	4.0392	-	7471B	PPB	02 May 2024 14:08:33	U	SMPL
P2330-01 - 1	B-1(0.5-1.5)	7504	1.4152	-	7471B	PPB	02 May 2024 14:10:49	U	SMPL
P2330-03 - 1	D-1(0.5-1.5)	7904	1.4911	-	7471B	PPB	02 May 2024 14:13:09	U	SMPL
P2330-05 - 1	F-1(0.5-1.5)	32088	6.0789	-	7471B	PPB	02 May 2024 14:15:27	U	SMPL
P2330-07 - 1	H-1(0.5-1.5)	6945	1.3092	-	7471B	PPB	02 May 2024 14:17:46	U	SMPL
P2330-09 - 1	C-2(0.5-1.5)	5874	1.1060	-	7471B	PPB	02 May 2024 14:20:07	U	SMPL
P2330-11 - 1	E-2(0.5-1.5)	6686	1.2600	-	7471B	PPB	02 May 2024 14:22:26	U	SMPL
P2330-13 - 1	G-2(0.5-1.5)	7682	1.4490	-	7471B	PPB	02 May 2024 14:24:45	U	SMPL
P2330-15 - 1	C-3(0.5-1.5)	4405	0.8273	-	7471B	PPB	02 May 2024 14:27:05	U	SMPL
P2330-17 - 1	F-3(0.5-1.5)	7183	1.3543	-	7471B	PPB	02 May 2024 14:29:23	U	SMPL
CCV10 - 1	CCV10	24669	4.6715	-	7471B	PPB	02 May 2024 14:33:56	U	SMPL
CCB10 - 1	CCB10	72	0.0053	-	7471B	PPB	02 May 2024 14:36:13	U	SMPL
P2330-19 - 1	E-4(0.5-1.5)	8189	1.5452	-	7471B	PPB	02 May 2024 14:38:32	U	SMPL
P2330-21 - 1	H-4(0.5-1.5)	8121	1.5323	-	7471B	PPB	02 May 2024 14:45:42	U	SMPL
P2330-21DUP - 1	H-4(0.5-1.5)DUP	7598	1.4330	-	7471B	PPB	02 May 2024 14:47:59	U	SMPL
P2330-21MS - 1	H-4(0.5-1.5)MS	25180	4.7684	-	7471B	PPB	02 May 2024 14:53:21	U	SMPL
P2330-21MSD - 1	H-4(0.5-1.5)MSD	26421	5.0038	-	7471B	PPB	02 May 2024 14:55:37	U	SMPL
P2340-01LX5 - 1		632	0.1116	-	7471B	PPB	02 May 2024 14:57:56	U	SMPL
P2340-01A - 1		24813	4.6988	-	7471B	PPB	02 May 2024 15:00:16	U	SMPL
P2330-21LX5 - 1		1639	0.3026	-	7471B	PPB	02 May 2024 15:02:33	U	SMPL
P2330-21A - 1		28580	5.4134	-	7471B	PPB	02 May 2024 15:04:55	U	SMPL
CCV11 - 1	CCV11	27086	5.1300	-	7471B	PPB	02 May 2024 15:07:10	U	SMPL
CCB11 - 1	CCB11	90	0.0088	-	7471B	PPB	02 May 2024 15:09:30	U	SMPL