


LB130718

SFAM01.1

INSTRUMENT ID: CV2

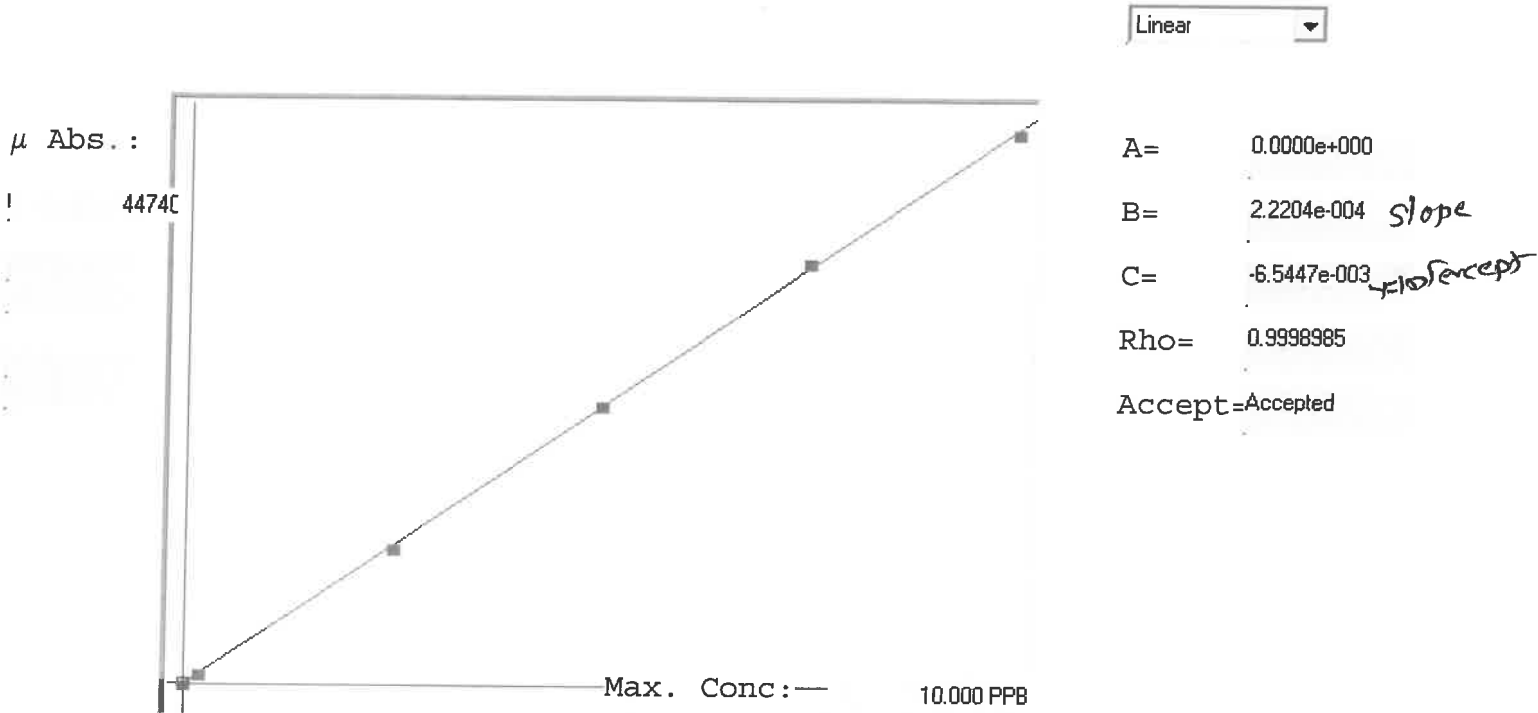

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	g/dl)
0.00	0.000	0.005	0.005	50	0.000	50					1
0.05	0.050					442	0				-3
0.20	0.200	0.195	-0.005	907	0.0 %	907					-2
2.50	2.500	2.460	-0.040	11110	0.0 %	11110					0
5.00	5.000	5.015	0.015	22615	0.0 %	22615					1
7.50	7.500	7.598	0.098	34246	0.0 %	34246					-1
10.0	10.000	9.928	-0.072	44740	0.0 %	44740					

LB130718

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	50	-		0 SFAM01.1	PPB	5/10/2024 14:13	Std
	0.2 S01	907	-		0.2 SFAM01.1	PPB	5/10/2024 14:15	Std
	2.5 S02	11110	-		2.5 SFAM01.1	PPB	5/10/2024 14:17	Std
	5 S03	22615	-		5 SFAM01.1	PPB	5/10/2024 14:20	Std
	7.5 S04	34246	-		7.5 SFAM01.1	PPB	5/10/2024 14:22	Std
	10 S05	44740	-		10 SFAM01.1	PPB	5/10/2024 14:24	Std
ICV042	ICV042	18025	3.9958 -		SFAM01.1	PPB	5/10/2024 14:27	SMPL
ICB042	ICB042	-288	-0.0705 -		SFAM01.1	PPB	5/10/2024 14:29	SMPL
CCV064	CCV064	22897	5.0776 -		SFAM01.1	PPB	5/10/2024 14:32	SMPL
CCB064	CCB064	-291	-0.0712 -		SFAM01.1	PPB	5/10/2024 14:34	SMPL
PB160864BL	PBW864	-21	-0.0112 -		SFAM01.1	PPB	5/10/2024 14:36	SMPL
PB160793TB	LEB793	52	0.005 -		SFAM01.1	PPB	5/10/2024 14:39	SMPL
P2376-01	E0Y34	128	0.0219 -		SFAM01.1	PPB	5/10/2024 14:41	SMPL
P2376-03	E0Y34D	120	0.0201 -		SFAM01.1	PPB	5/10/2024 14:43	SMPL
P2376-04	E0Y34S	4706	1.0384 -		SFAM01.1	PPB	5/10/2024 14:45	SMPL
PB160865BL	PBW865	-26	-0.0123 -		SFAM01.1	PPB	5/10/2024 14:48	SMPL
PB160798TB	LEB798	46	0.0037 -		SFAM01.1	PPB	5/10/2024 14:50	SMPL
P2376-02	E0Y33	148	0.0263 -		SFAM01.1	PPB	5/10/2024 14:52	SMPL
CCV065	CCV065	22234	4.9304 -		SFAM01.1	PPB	5/10/2024 14:54	SMPL
CCB065	CCB065	-238	-0.0594 -		SFAM01.1	PPB	5/10/2024 14:57	SMPL