


7470A

INSTRUMENT ID: CVZ

Linear

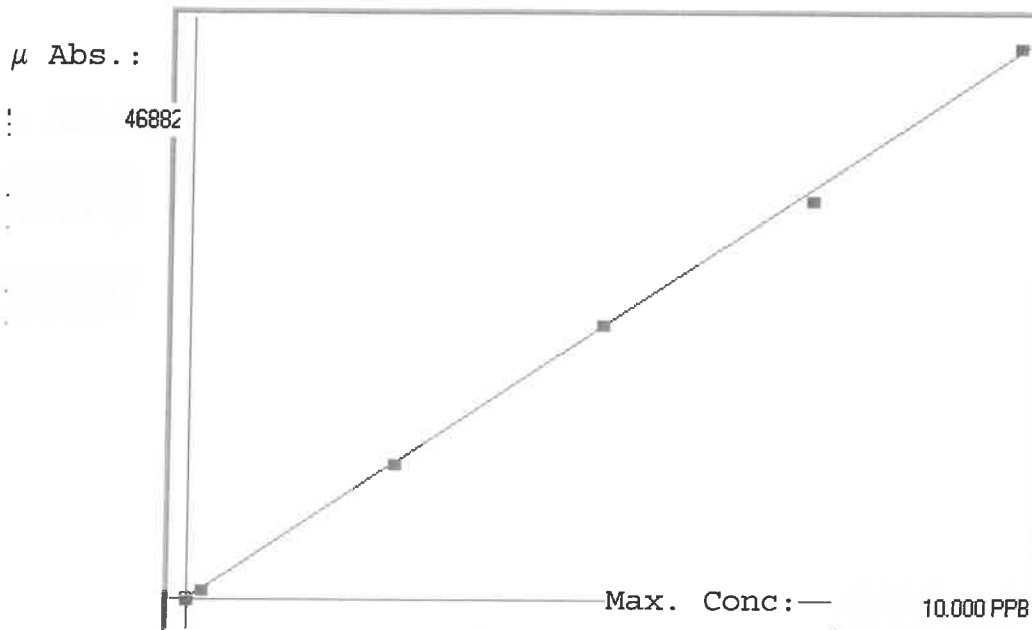

A= 0.0000e+000

B= 2.1527e-004

C= 9.3126e-003

Rho= 0.9997378

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/10
0.0	0.000	0.014	0.014	22	0.000	22	0				1
0.2	0.200	0.203	0.003	902	0.0 %	902					2
2.5	2.500	2.512	0.012	11624	0.0 %	11624					6
5.0	5.000	5.043	0.043	23384	0.0 %	23384					1
7.5	7.500	7.326	-0.174	33988	0.0 %	33988					2
10.0	10.000	10.102	0.102	46882	0.0 %	46882					1

LB130723 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 10 May 2024 16:00:21

Sample ID	Extended ID	µ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	22	-	0.0000	7470A	PPB	10 May 2024 16:00:32	S	Std
0.2 - 1	50.2	902	-	0.2000	7470A	PPB	10 May 2024 16:02:50	S	Std
2.5 - 1	52.5	11624	-	2.5000	7470A	PPB	10 May 2024 16:05:07	S	Std
5.0 - 1	55	23384	-	5.0000	7470A	PPB	10 May 2024 16:07:23	S	Std
7.5 - 1	57.5	33988	-	7.5000	7470A	PPB	10 May 2024 16:09:41	S	Std
10.0 - 1	59.0	46882	-	10.0000	7470A	PPB	10 May 2024 16:11:59	S	Std
ICV43 - 1	ICV43	17898	3.8618	-	7470A	PPB	10 May 2024 16:14:51	U	SMPL
ICB43 - 1	ICB43	-374	-0.0712	-	7470A	PPB	10 May 2024 16:17:07	U	SMPL
CCV66 - 1	CCV66	23740	5.1199	-	7470A	PPB	10 May 2024 16:19:24	U	SMPL
CCB66 - 1	CCB66	-365	-0.0693	-	7470A	PPB	10 May 2024 16:21:39	U	SMPL
CRA - 1	CRA	805	0.1826	-	7470A	PPB	10 May 2024 16:23:57	U	SMPL
HighStd - 1	HighStd	47241	10.1789	-	7470A	PPB	10 May 2024 16:26:12	U	SMPL
ChkStd - 1	ChkStd	30388	6.5510	-	7470A	PPB	10 May 2024 16:28:28	U	SMPL
PB160826BL - 1	PBW	-76	-0.0070	-	7470A	PPB	10 May 2024 16:33:25	U	SMPL
PB160826BS - 1	LCSW	18031	3.8909	-	7470A	PPB	10 May 2024 16:35:40	U	SMPL
P2375-02 - 1	WC-A-COMP	-267	-0.0482	-	7470A	PPB	10 May 2024 16:37:57	U	SMPL
P2396-01 - 1	149TH-ST-21-PPE	-63	-0.0042	-	7470A	PPB	10 May 2024 16:40:17	U	SMPL
P2396-02 - 1	149TH-ST-22-POLY	-17	0.0057	-	7470A	PPB	10 May 2024 16:42:34	U	SMPL
P2398-04 - 1	WC-KK	-11	0.0069	-	7470A	PPB	10 May 2024 16:44:51	U	SMPL
P2411-04 - 1	WCS-TPA	23	0.0143	-	7470A	PPB	10 May 2024 16:47:06	U	SMPL
CCV67 - 1	CCV67	23851	5.1437	-	7470A	PPB	10 May 2024 16:49:22	U	SMPL
CCB67 - 1	CCB67	-314	-0.0583	-	7470A	PPB	10 May 2024 16:51:37	U	SMPL
P2413-04 - 1	WC-CC	71	0.0246	-	7470A	PPB	10 May 2024 16:53:55	U	SMPL
P2413-08 - 1	WC-EE	194	0.0511	-	7470A	PPB	10 May 2024 16:56:10	U	SMPL
P2414-02 - 1	1011UMR-SS004-0212-01	2	0.0097	-	7470A	PPB	10 May 2024 16:58:26	U	SMPL
P2415-02 - 1	1011UMR-SS005-0212-01	55	0.0212	-	7470A	PPB	10 May 2024 17:00:42	U	SMPL
P2415-02DUP - 1	1011UMR-SS005-0212-01DUP	22	0.0140	-	7470A	PPB	10 May 2024 17:02:57	U	SMPL
P2415-02MS - 1	1011UMR-SS005-0212-01MS	16952	3.6586	-	7470A	PPB	10 May 2024 17:05:14	U	SMPL
P2415-02MSD - 1	1011UMR-SS005-0212-01MSD	17893	3.8612	-	7470A	PPB	10 May 2024 17:07:30	U	SMPL
PB160758TB - 1	PB160758TB	-312	-0.0579	-	7470A	PPB	10 May 2024 17:09:49	U	SMPL
P2415-02LX5 - 1		92	0.0291	-	7470A	PPB	10 May 2024 17:12:08	U	SMPL
P2415-02A - 1		18266	3.9415	-	7470A	PPB	10 May 2024 17:14:24	U	SMPL
CCV68 - 1	CCV68	24096	5.1965	-	7470A	PPB	10 May 2024 17:16:39	U	SMPL
CCB68 - 1	CCB68	-385	-0.0736	-	7470A	PPB	10 May 2024 17:18:57	U	SMPL