


LB130759

7470A

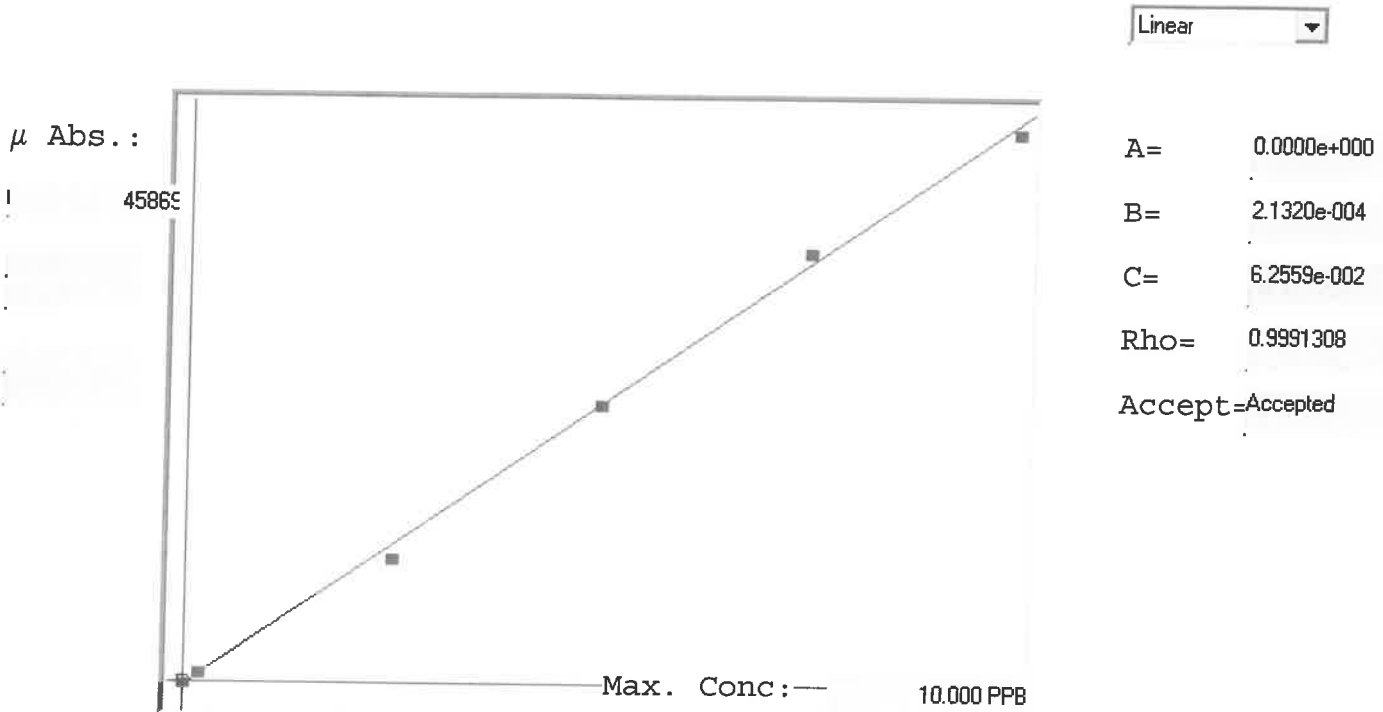

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/00
0.0	0.000	0.066	0.066	18	0.000	18	0				-
0.2	0.200	0.240	0.040	830	0.0 %	830					20
2.5	2.500	2.275	-0.225	10379	0.0 %	10379					-9
5.0	5.000	5.033	0.033	23315	0.0 %	23315					1
7.5	7.500	7.744	0.244	36028	0.0 %	36028					3
10.0	10.000	9.842	-0.158	45869	0.0 %	45869					-2

LB130759 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 14 May 2024 15:12:26

Sample ID	Extended ID	µ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	18	-	0.0000	7470A	PPB	14 May 2024 15:37:53	S	Std
0.2 - 1	50.2	830	-	0.2000	7470A	PPB	14 May 2024 15:40:10	S	Std
2.5 - 1	52.5	10379	-	2.5000	7470A	PPB	14 May 2024 15:42:27	S	Std
5.0 - 1	55	23315	-	5.0000	7470A	PPB	14 May 2024 15:44:44	S	Std
7.5 - 1	55.5	36028	-	7.5000	7470A	PPB	14 May 2024 15:47:02	S	Std
10.0 - 1	58	45869	-	10.0000	7470A	PPB	14 May 2024 15:49:21	S	Std
ICV47 - 1	ICV47	18065	3.9140	-	7470A	PPB	14 May 2024 15:52:28	U	SMPL
ICB47 - 1	ICB47	-582	-0.0615	-	7470A	PPB	14 May 2024 15:54:44	U	SMPL
CCV78 - 1	CCV78	23248	5.0190	-	7470A	PPB	14 May 2024 15:57:01	U	SMPL
CCB78 - 1	CCB78	-516	-0.0475	-	7470A	PPB	14 May 2024 15:59:15	U	SMPL
CRA - 1	CRA	743	0.2210	-	7470A	PPB	14 May 2024 16:01:32	U	SMPL
HighStd - 1	HighStd	45307	9.7220	-	7470A	PPB	14 May 2024 16:03:47	U	SMPL
ChkStd - 1	ChkStd	32863	7.0689	-	7470A	PPB	14 May 2024 16:06:02	U	SMPL
PB160926BL - 1	PBW	-620	-0.0696	-	7470A	PPB	14 May 2024 16:08:21	U	SMPL
PB160926BS - 1	LCSW	16016	3.4771	-	7470A	PPB	14 May 2024 16:13:16	U	SMPL
P2437-08 - 1	WAREHOUSE-TOTE-WATER	5266	1.1853	-	7470A	PPB	14 May 2024 16:15:33	U	SMPL
P2440-03 - 1	EQ-TANK-CONTAINMENT-PIT	-308	-0.0031	-	7470A	PPB	14 May 2024 16:17:53	U	SMPL
P2440-03DUP - 1	EQ-TANK-CONTAINMENT-PITDUP	-10	0.0604	-	7470A	PPB	14 May 2024 16:20:12	U	SMPL
P2440-03MS - 1	EQ-TANK-CONTAINMENT-PITMS	15334	3.3317	-	7470A	PPB	14 May 2024 16:22:29	U	SMPL
P2440-03MSD - 1	EQ-TANK-CONTAINMENT-PITMSD	15405	3.3469	-	7470A	PPB	14 May 2024 16:27:16	U	SMPL
CCV79 - 1	CCV79	22117	4.7779	-	7470A	PPB	14 May 2024 16:29:31	U	SMPL
CCB79 - 1	CCB79	-332	-0.0082	-	7470A	PPB	14 May 2024 16:31:49	U	SMPL
P2441-01 - 1	INTERMEDIATE-VAULT	-143	0.0321	-	7470A	PPB	14 May 2024 16:34:06	U	SMPL
P2441-04 - 1	FRAGILE-WETLAND-NORTH	-43	0.0534	-	7470A	PPB	14 May 2024 16:36:21	U	SMPL
P2441-07 - 1	SEEPAGE-PIT	43	0.0717	-	7470A	PPB	14 May 2024 16:38:37	U	SMPL
P2449-05 - 1	1011UMR-RB240508-01	-13	0.0596	-	7470A	PPB	14 May 2024 16:40:53	U	SMPL
P2450-01 - 1	1011UMR-RB240507-01	-28	0.0566	-	7470A	PPB	14 May 2024 16:43:09	U	SMPL
P2452-02 - 1	TT-060-IDWGW-20240509	3831	0.8793	-	7470A	PPB	14 May 2024 16:45:25	U	SMPL
P2452-03 - 1	TT-061-IDWGW-20240509	574	0.1849	-	7470A	PPB	14 May 2024 16:47:42	U	SMPL
P2454-01 - 1	SP25-06-20240510-WC	11289	2.4694	-	7470A	PPB	14 May 2024 16:50:02	U	SMPL
P2458-05 - 1	34790	4982	1.1247	-	7470A	PPB	14 May 2024 16:52:20	U	SMPL
CCV80 - 1	CCV80	22279	4.8124	-	7470A	PPB	14 May 2024 16:54:38	U	SMPL
CCB80 - 1	CCB80	-160	0.0284	-	7470A	PPB	14 May 2024 16:56:56	U	SMPL
P2440-03LX5 - 1		-12	0.0600	-	7470A	PPB	14 May 2024 16:59:14	U	SMPL
P2440-03A - 1		16632	3.6085	-	7470A	PPB	14 May 2024 17:01:30	U	SMPL
CCV81 - 1	CCV81	21409	4.6269	-	7470A	PPB	14 May 2024 17:06:25	U	SMPL
CCB81 - 1	CCB81	-331	-0.0080	-	7470A	PPB	14 May 2024 17:08:40	U	SMPL