


LB130819

7471B

INSTRUMENT ID: CV2

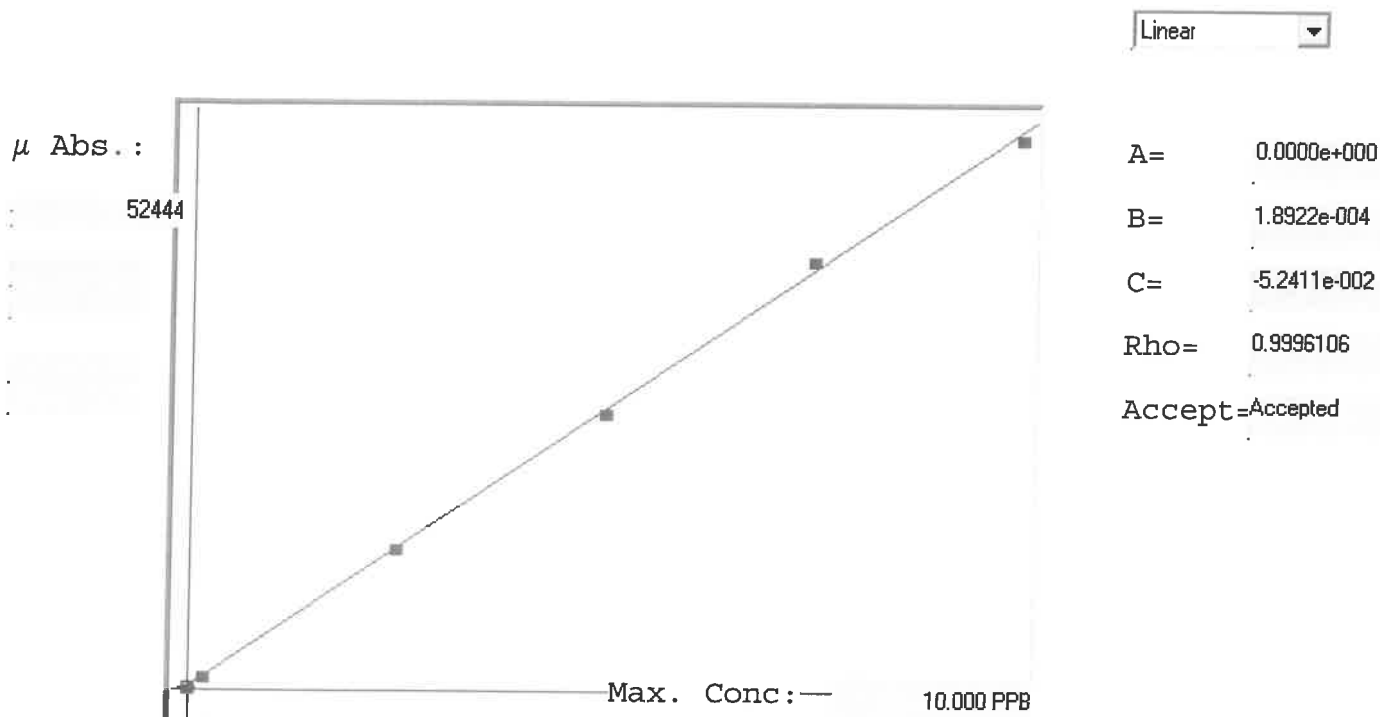

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/bD
0.0	0.000	-0.011	-0.011	220	0.000	220					0/00
0.2	0.200	0.195	-0.005	1307	0.0 %	1307					-3
2.5	2.500	2.505	0.005	13517	0.0 %	13517					0
5.0	5.000	4.933	-0.067	26348	0.0 %	26348					-1
7.5	7.500	7.706	0.206	41001	0.0 %	41001					-3
10.0	10.000	9.871	-0.129	52444	0.0 %	52444					1

LB130819 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 17 May 2024 14:33:47

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	30	220	-	0.0000	7471B	PPB	17 May 2024 14:38:05	S	Std
0.2 - 1	50.2	1307	-	0.2000	7471B	PPB	17 May 2024 14:40:22	S	Std
2.5 - 1	52.5	13517	-	2.5000	7471B	PPB	17 May 2024 14:42:39	S	Std
5.0 - 1	55	26348	-	5.0000	7471B	PPB	17 May 2024 14:44:56	S	Std
7.5 - 1	57.5	41001	-	7.5000	7471B	PPB	17 May 2024 14:47:15	S	Std
10.0 - 1	510	52444	-	10.0000	7471B	PPB	17 May 2024 14:49:36	S	Std
ICV55 - 1	ICV55	20831	3.8893	-	7471B	PPB	17 May 2024 14:52:50	U	SMPL
ICB55 - 1	ICB55	-118	-0.0747	-	7471B	PPB	17 May 2024 14:55:05	U	SMPL
CCV06 - 1	CCV06	25922	4.8527	-	7471B	PPB	17 May 2024 14:57:25	U	SMPL
CCB06 - 1	CCB06	-127	-0.0764	-	7471B	PPB	17 May 2024 14:59:40	U	SMPL
CRA - 1	CRA	1263	0.1866	-	7471B	PPB	17 May 2024 15:02:01	U	SMPL
HighStd - 1	HighStd	51590	9.7097	-	7471B	PPB	17 May 2024 15:04:16	U	SMPL
ChkStd - 1	ChkStd	37689	7.0793	-	7471B	PPB	17 May 2024 15:06:31	U	SMPL
PB160984BL - 1	PB160984BL	229	-0.0091	-	7471B	PPB	17 May 2024 15:08:59	U	SMPL
PB160984BS - 1	PB160984BS	24557	4.5944	-	7471B	PPB	17 May 2024 15:11:23	U	SMPL
P2494-01 - 1	1	8861	1.6243	-	7471B	PPB	17 May 2024 15:13:39	U	SMPL
P2494-02 - 1	2	3257	0.5639	-	7471B	PPB	17 May 2024 15:15:59	U	SMPL
P2494-03 - 1	3	2236	0.3707	-	7471B	PPB	17 May 2024 15:18:18	U	SMPL
P2494-04 - 1	4	4092	0.7219	-	7471B	PPB	17 May 2024 15:20:37	U	SMPL
P2494-05 - 1	5	5495	0.9874	-	7471B	PPB	17 May 2024 15:22:54	U	SMPL
CCV07 - 1	CCV07	24431	4.5705	-	7471B	PPB	17 May 2024 15:25:11	U	SMPL
CCB07 - 1	CCB07	20	-0.0486	-	7471B	PPB	17 May 2024 15:27:29	U	SMPL
P2494-06 - 1	6	4165	0.7357	-	7471B	PPB	17 May 2024 15:29:47	U	SMPL
P2494-07 - 1	7	3336	0.5788	-	7471B	PPB	17 May 2024 15:32:03	U	SMPL
P2494-08 - 1	8	1433	0.2187	-	7471B	PPB	17 May 2024 15:34:20	U	SMPL
P2494-09 - 1	9	1075	0.1510	-	7471B	PPB	17 May 2024 15:36:37	U	SMPL
P2494-10 - 1	10	1223	0.1790	-	7471B	PPB	17 May 2024 15:38:54	U	SMPL
P2494-11 - 1	11	3685	0.6449	-	7471B	PPB	17 May 2024 15:41:11	U	SMPL
P2494-12 - 1	12	4029	0.7100	-	7471B	PPB	17 May 2024 15:43:27	U	SMPL
P2494-13 - 1	13	2496	0.4199	-	7471B	PPB	17 May 2024 15:45:46	U	SMPL
P2494-14 - 1	14	1198	0.1743	-	7471B	PPB	17 May 2024 15:48:04	U	SMPL
P2494-15 - 1	15	2253	0.3739	-	7471B	PPB	17 May 2024 15:50:21	U	SMPL
CCV08 - 1	CCV08	25109	4.6988	-	7471B	PPB	17 May 2024 15:52:36	U	SMPL
CCB08 - 1	CCB08	36	-0.0456	-	7471B	PPB	17 May 2024 15:54:53	U	SMPL
P2494-16 - 1	16	11978	2.2141	-	7471B	PPB	17 May 2024 15:57:12	U	SMPL
P2494-17 - 1	17	548	0.0513	-	7471B	PPB	17 May 2024 15:59:28	U	SMPL
P2494-18 - 1	18	1074	0.1508	-	7471B	PPB	17 May 2024 16:01:46	U	SMPL
P2494-20 - 1	19	1200	0.1747	-	7471B	PPB	17 May 2024 16:04:02	U	SMPL
P2494-20DUP - 1	19DUP	817	0.1022	-	7471B	PPB	17 May 2024 16:06:18	U	SMPL
P2494-20MS - 1	19MS	17750	3.3063	-	7471B	PPB	17 May 2024 16:08:35	U	SMPL
P2494-20MSD - 1	19MSD	17804	3.3165	-	7471B	PPB	17 May 2024 16:10:52	U	SMPL
PB160985BL - 1	PB160985BL	367	0.0170	-	7471B	PPB	17 May 2024 16:13:12	U	SMPL
PB160985BS - 1	PB160985BS	21266	3.9716	-	7471B	PPB	17 May 2024 16:15:33	U	SMPL
P2495-01 - 1	RT-3463	6154	1.1121	-	7471B	PPB	17 May 2024 16:17:48	U	SMPL
CCV09 - 1	CCV09	25358	4.7459	-	7471B	PPB	17 May 2024 16:20:07	U	SMPL
CCB09 - 1	CCB09	-37	-0.0594	-	7471B	PPB	17 May 2024 16:22:25	U	SMPL
P2495-01DUP - 1	RT-3463DUP	6310	1.1416	-	7471B	PPB	17 May 2024 16:24:47	U	SMPL
P2495-01MS - 1	RT-3463MS	29272	5.4866	-	7471B	PPB	17 May 2024 16:27:03	U	SMPL
P2495-01MSD - 1	RT-3463MSD	28688	5.3761	-	7471B	PPB	17 May 2024 16:29:21	U	SMPL
P2498-01 - 1	OK-01-051524	2243	0.3720	-	7471B	PPB	17 May 2024 16:31:43	U	SMPL
P2500-01 - 1	B-112-SB01	44933	8.4500	-	7471B	PPB	17 May 2024 16:34:06	U	SMPL
P2500-02 - 1	B-112-SB02	4421	0.7842	-	7471B	PPB	17 May 2024 16:36:23	U	SMPL
P2511-03 - 1	510-CD	2967	0.5090	-	7471B	PPB	17 May 2024 16:38:49	U	SMPL
P2511-04 - 1	665	644	0.0694	-	7471B	PPB	17 May 2024 16:41:07	U	SMPL
P2512-01 - 1	WCS-TPJ	7591	1.3840	-	7471B	PPB	17 May 2024 16:43:26	U	SMPL
P2512-05 - 1	WCS-TPI	9439	1.7337	-	7471B	PPB	17 May 2024 16:45:41	U	SMPL
CCV10 - 1	CCV10	25094	4.6960	-	7471B	PPB	17 May 2024 16:48:00	U	SMPL
CCB10 - 1	CCB10	-62	-0.0641	-	7471B	PPB	17 May 2024 16:50:18	U	SMPL
P2513-01 - 1	TP-13	7106	1.2922	-	7471B	PPB	17 May 2024 16:52:39	U	SMPL
P2513-04 - 1	TP-14	1511	0.2335	-	7471B	PPB	17 May 2024 16:54:55	U	SMPL
P2513-07 - 1	TP-15	1669	0.2634	-	7471B	PPB	17 May 2024 16:57:13	U	SMPL
P2513-10 - 1	TP-16	1935	0.3137	-	7471B	PPB	17 May 2024 16:59:28	U	SMPL
P2513-13 - 1	TP-17	682	0.0766	-	7471B	PPB	17 May 2024 17:01:46	U	SMPL
P2494-20LX5 - 1		312	0.0066	-	7471B	PPB	17 May 2024 17:04:02	U	SMPL
P2494-20A - 1		20227	3.7750	-	7471B	PPB	17 May 2024 17:06:19	U	SMPL
P2495-01LX5 - 1		1047	0.1457	-	7471B	PPB	17 May 2024 17:11:26	U	SMPL
P2495-01A - 1		29182	5.4695	-	7471B	PPB	17 May 2024 17:13:43	U	SMPL
CCV11 - 1	CCV11	25140	4.7047	-	7471B	PPB	17 May 2024 17:15:59	U	SMPL
CCB11 - 1	CCB11	-182	-0.0869	-	7471B	PPB	17 May 2024 17:18:22	U	SMPL