


LB130832

7470A

INSTRUMENT ID: CV1

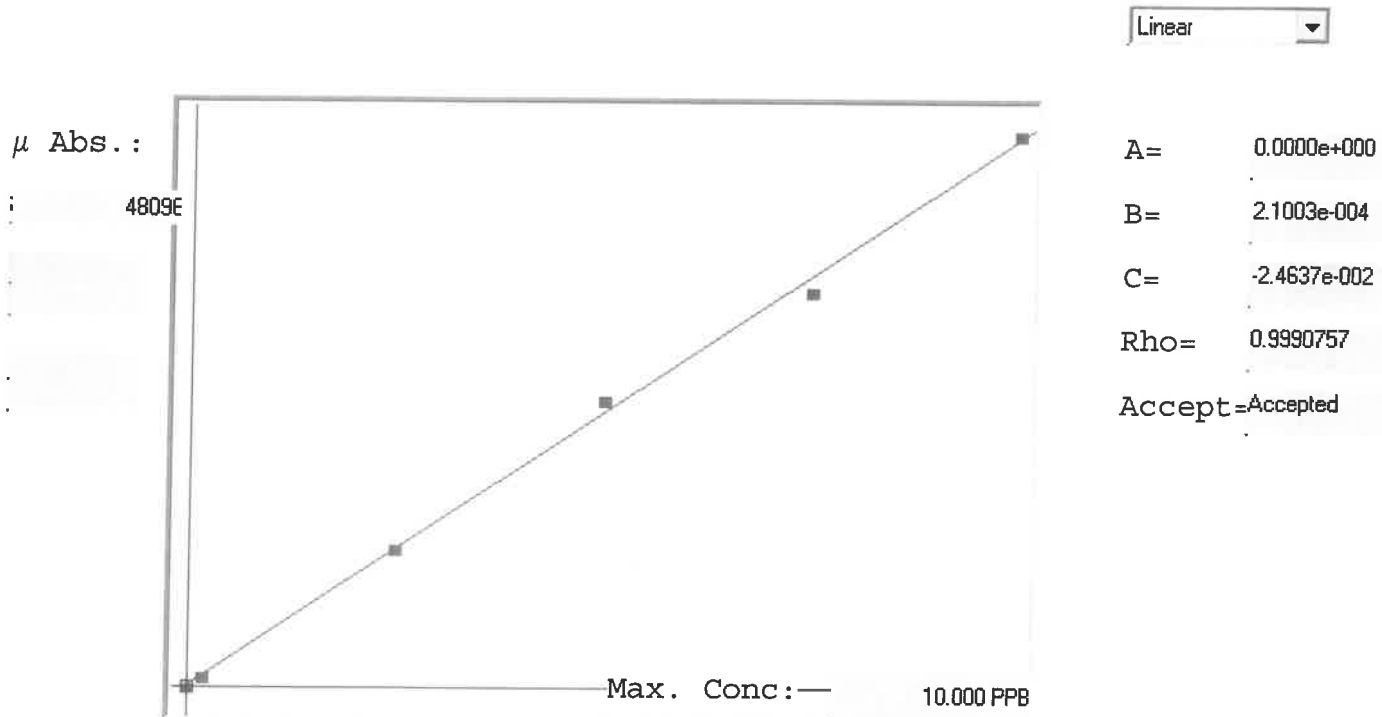

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	Δ/1)
0.0	0.000	-0.016	-0.016	43	0.000	43	0				1
0.2	0.200	0.182	-0.018	986	0.0 %	986					-9
2.5	2.500	2.493	-0.007	11986	0.0 %	11986					0
5.0	5.000	5.250	0.250	25113	0.0 %	25113					5
7.5	7.500	7.214	-0.286	34463	0.0 %	34463					-4
10.0	10.000	10.077	0.077	48096	0.0 %	48096					1

LB130832 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 20 May 2024 13:03:05

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	80	43	-	0.0000	7470A	PPB	20 May 2024 13:43:15	S	Std
0.2 - 1	50-2	986	-	0.2000	7470A	PPB	20 May 2024 13:47:07	S	Std
2.5 - 1	52-5	11986	-	2.5000	7470A	PPB	20 May 2024 13:49:24	S	Std
5.0 - 1	55	25113	-	5.0000	7470A	PPB	20 May 2024 13:51:40	S	Std
7.5 - 1	57-5	34463	-	7.5000	7470A	PPB	20 May 2024 13:53:59	S	Std
10.0 - 1	510	48096	-	10.0000	7470A	PPB	20 May 2024 14:01:34	S	Std
ICV56 - 1	ICV56	19387	4.0472	-	7470A	PPB	20 May 2024 14:04:21	U	SMPL
ICB56 - 1	ICB56	425	0.0646	-	7470A	PPB	20 May 2024 14:09:20	U	SMPL
CCV12 - 1	CCV12	23417	4.8936	-	7470A	PPB	20 May 2024 14:11:35	U	SMPL
CCB12 - 1	CCB12	150	0.0069	-	7470A	PPB	20 May 2024 14:13:50	U	SMPL
CRA - 1	CRA	1239	0.2356	-	7470A	PPB	20 May 2024 14:20:51	U	SMPL
HighStd - 1	HighStd	48287	10.1171	-	7470A	PPB	20 May 2024 14:23:06	U	SMPL
ChkStd - 1	ChkStd	33489	7.0090	-	7470A	PPB	20 May 2024 14:25:22	U	SMPL
PB160990BL - 1	PBW	300	0.0384	-	7470A	PPB	20 May 2024 14:32:52	U	SMPL
PB160990BS - 1	LCSW	17924	3.7399	-	7470A	PPB	20 May 2024 14:35:08	U	SMPL
P2512-04 - 1	WCS-TPJ	-48	-0.0347	-	7470A	PPB	20 May 2024 14:37:24	U	SMPL
P2512-08 - 1	WCS-TPI	240	0.0258	-	7470A	PPB	20 May 2024 14:39:43	U	SMPL
P2513-03 - 1	TP-13	404	0.0602	-	7470A	PPB	20 May 2024 14:42:00	U	SMPL
P2513-06 - 1	TP-14	380	0.0552	-	7470A	PPB	20 May 2024 14:44:17	U	SMPL
P2513-09 - 1	TP-15	149	0.0067	-	7470A	PPB	20 May 2024 14:46:32	U	SMPL
CCV13 - 1	CCV13	23218	4.8518	-	7470A	PPB	20 May 2024 14:48:47	U	SMPL
CCB13 - 1	CCB13	410	0.0615	-	7470A	PPB	20 May 2024 14:54:04	U	SMPL
P2513-12 - 1	TP-16	253	0.0285	-	7470A	PPB	20 May 2024 14:56:19	U	SMPL
P2513-15 - 1	TP-17	139	0.0046	-	7470A	PPB	20 May 2024 14:58:35	U	SMPL
P2518-04 - 1	WC-MH-MM	180	0.0132	-	7470A	PPB	20 May 2024 15:00:51	U	SMPL
P2518-08 - 1	WC-MH-LL	61	-0.0118	-	7470A	PPB	20 May 2024 15:03:07	U	SMPL
P2518-12 - 1	WC-MH-FF	468	0.0737	-	7470A	PPB	20 May 2024 15:05:23	U	SMPL
P2518-12DUP - 1	WC-MH-FFDUP	76	-0.0087	-	7470A	PPB	20 May 2024 15:07:39	U	SMPL
P2518-12MS - 1	WC-MH-FFMS	15979	3.3314	-	7470A	PPB	20 May 2024 15:09:56	U	SMPL
P2518-12MSD - 1	WC-MH-FFMSD	16892	3.5232	-	7470A	PPB	20 May 2024 15:12:13	U	SMPL
PB160991BL - 1	PBW	201	0.0176	-	7470A	PPB	20 May 2024 15:14:31	U	SMPL
PB160991BS - 1	LCSW	16725	3.4881	-	7470A	PPB	20 May 2024 15:16:50	U	SMPL
CCV14 - 1	CCV14	25874	5.4097	-	7470A	PPB	20 May 2024 15:19:05	U	SMPL
CCB14 - 1	CCB14	113	-0.0009	-	7470A	PPB	20 May 2024 15:21:21	U	SMPL
P2472-01 - 1	WC-EX-1	370	0.0531	-	7470A	PPB	20 May 2024 15:23:39	U	SMPL
P2472-01DUP - 1	WC-EX-1DUP	396	0.0585	-	7470A	PPB	20 May 2024 15:25:55	U	SMPL
P2472-01MS - 1	WC-EX-1MS	16009	3.3377	-	7470A	PPB	20 May 2024 15:28:10	U	SMPL
P2472-01MSD - 1	WC-EX-1MSD	18299	3.8187	-	7470A	PPB	20 May 2024 15:30:26	U	SMPL
PB161007BL - 1	PBW	-220	-0.0708	-	7470A	PPB	20 May 2024 15:32:45	U	SMPL
PB161007BS - 1	LCSW	17861	3.7267	-	7470A	PPB	20 May 2024 15:35:03	U	SMPL
P2511-07 - 1	510-AB	185	0.0142	-	7470A	PPB	20 May 2024 15:37:19	U	SMPL
P2511-07DUP - 1	510-ABDUP	392	0.0577	-	7470A	PPB	20 May 2024 15:39:38	U	SMPL
P2511-07MS - 1	510-ABMS	14574	3.0363	-	7470A	PPB	20 May 2024 15:41:54	U	SMPL
P2511-07MSD - 1	510-ABMSD	16876	3.5198	-	7470A	PPB	20 May 2024 15:44:11	U	SMPL
CCV15 - 1	CCV15	23239	4.8562	-	7470A	PPB	20 May 2024 15:46:29	U	SMPL
CCB15 - 1	CCB15	-86	-0.0427	-	7470A	PPB	20 May 2024 15:48:48	U	SMPL
P2515-01 - 1	MW-1-DISS	-46	-0.0343	-	7470A	PPB	20 May 2024 15:51:06	U	SMPL
P2515-02 - 1	MW-2-DISS	105	-0.0026	-	7470A	PPB	20 May 2024 15:53:21	U	SMPL
PB160966TB - 1	PB160966TB	385	0.0562	-	7470A	PPB	20 May 2024 15:55:37	U	SMPL
PB160991TB - 1	PB160991TB	191	0.0155	-	7470A	PPB	20 May 2024 15:57:53	U	SMPL
P2518-12LX5 - 1		215	0.0205	-	7470A	PPB	20 May 2024 16:00:09	U	SMPL
P2518-12A - 1		19630	4.0982	-	7470A	PPB	20 May 2024 16:02:25	U	SMPL
P2472-01LX5 - 1		547	0.0902	-	7470A	PPB	20 May 2024 16:04:42	U	SMPL
P2472-01A - 1		19531	4.0774	-	7470A	PPB	20 May 2024 16:07:01	U	SMPL
P2511-07LX5 - 1		36	-0.0171	-	7470A	PPB	20 May 2024 16:09:18	U	SMPL
P2511-07A - 1		16847	3.5137	-	7470A	PPB	20 May 2024 16:11:36	U	SMPL
CCV16 - 1	CCV16	24198	5.0577	-	7470A	PPB	20 May 2024 16:13:52	U	SMPL
CCB16 - 1	CCB16	-291	-0.0858	-	7470A	PPB	20 May 2024 16:16:10	U	SMPL