


Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A

ident	concentratio tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio n HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-051324	5/13/2024 15:40		IZ/MA
STD2	0.4450	0.6690	0.6700	2.1990	0.5620	1.1310	3.4510	IC1-051324	5/13/2024 16:02		IZ/MA
STD3	0.8040	1.2260	1.2290	4.0910	1.0210	1.9980	6.1260	IC1-051324	5/13/2024 16:23		IZ/MA
STD4	1.0000	1.4810	1.4990	4.9540	1.2400	2.5220	7.4370	IC1-051324	5/13/2024 16:45		IZ/MA
STD5	1.9530	2.9200	2.8930	9.7290	2.4170	4.8420	14.4330	IC1-051324	5/13/2024 17:06		IZ/MA
STD6	3.9170	5.8890	5.8830	19.6980	4.9170	9.7880	29.2960	IC1-051324	5/13/2024 17:27		IZ/MA
STD7	5.0810	7.6150	7.6260	25.3280	6.3430	12.7180	37.7560	IC1-051324	5/13/2024 17:49		IZ/MA

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	11.2500	11.5000	11.6667	9.9500	12.4000	13.1000	15.0333
STD3	0.5000	2.1667	2.4167	2.2750	2.1000	-0.1000	2.1000
STD4	0.0000	-1.2667	-0.0667	-0.9200	-0.8000	0.8800	-0.8400
STD5	-2.3500	-2.6667	-3.5667	-2.7100	-3.3200	-3.1600	-3.7800
STD6	-2.0750	-1.8500	-1.9500	-1.5100	-1.6600	-2.1200	-2.3467
STD7	1.6200	1.5333	1.6800	1.3120	1.4880	1.7440	2.0432

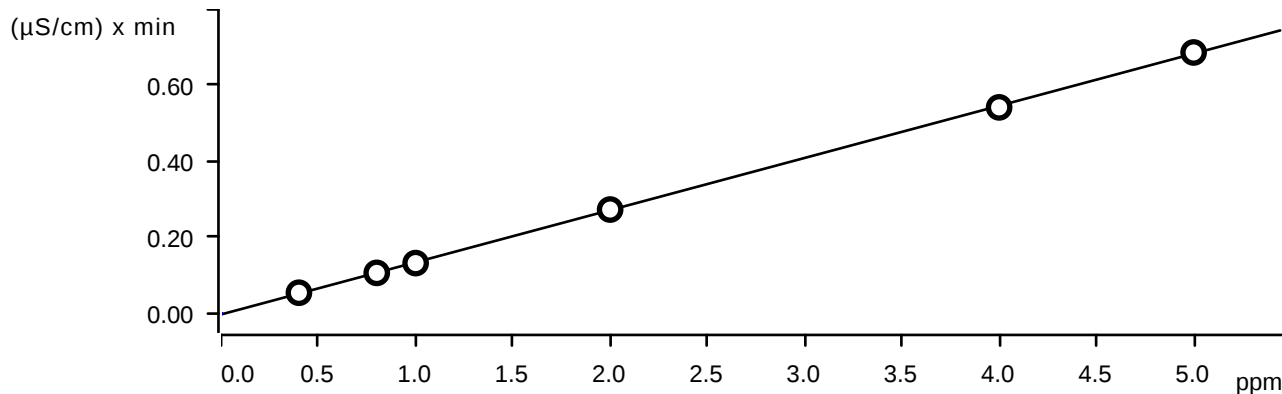
Fluoride (Anions)

Function: $A = -3.05003E-3 + 0.0137350 \times Q$

Relative standard deviation 1.034950 %

Correlation coefficient 0.999943


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.054	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.106	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.132	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.273	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.542	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.687	Std 7	2024-04-13 01:04:41 UTC-4	used

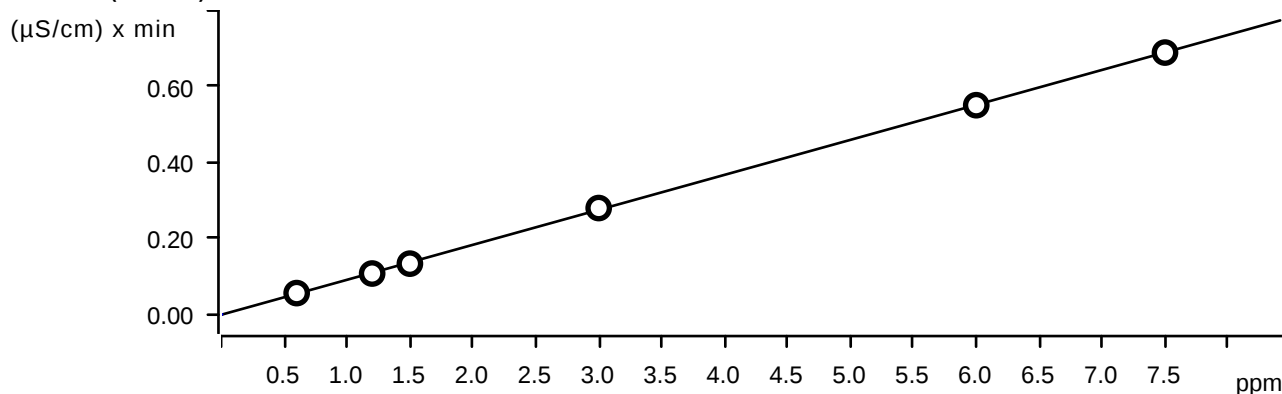Chloride (Anions)

Function: $A = -1.03082E-3 + 9.21146E-3 \times Q$

Relative standard deviation 1.071537 %
Correlation coefficient 0.999938


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.056	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.108	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.134	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.280	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.551	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.689	Std 7	2024-04-13 01:04:41 UTC-4	used

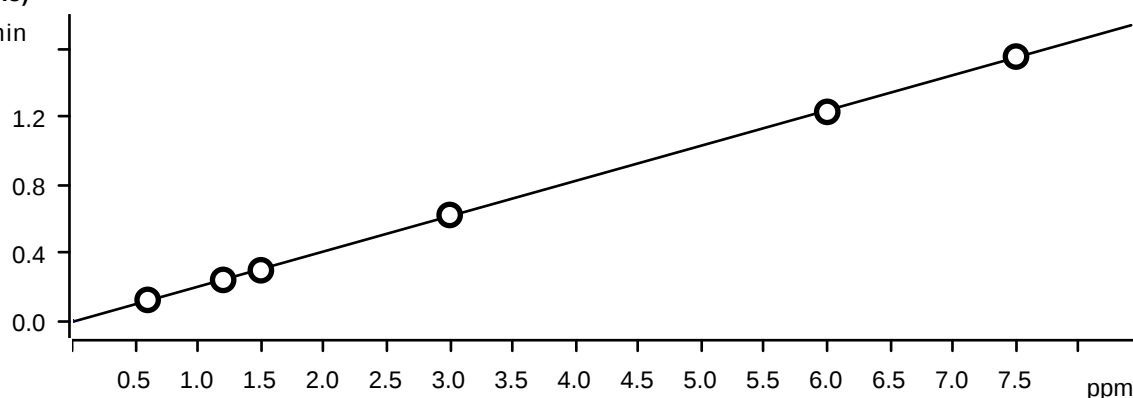Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ 

Function: $A = -8.19751E-3 + 0.0207534 \times Q$
Relative standard deviation 1.139145 %
Correlation coefficient 0.999931

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.122	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.239	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.296	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.621	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.228	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.554	Std 7	2024-04-13 01:04:41 UTC-4	used


Bromide (Anions)

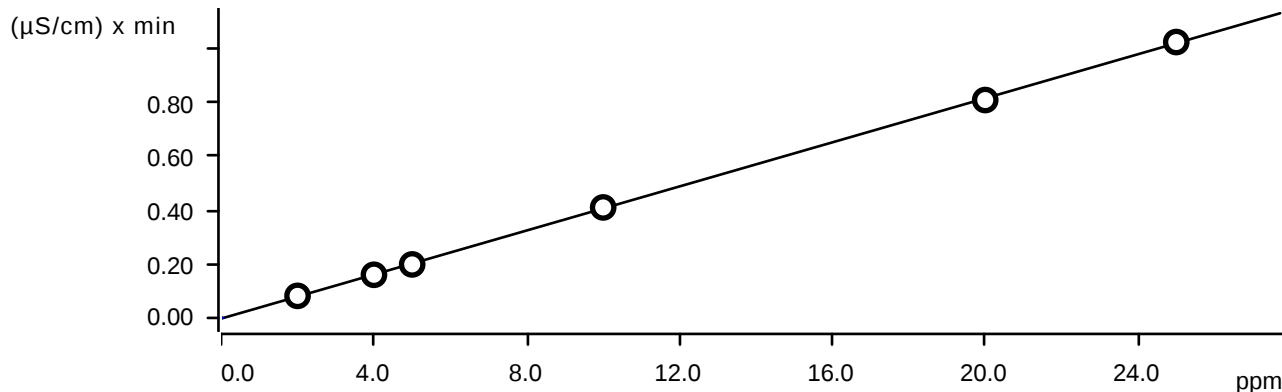

Function: $A = -2.93159E-3 + 4.09511E-3 \times Q$
 Relative standard deviation: 1.087762 %
 Correlation coefficient: 0.999936

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.082	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.160	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.199	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.410	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.810	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.025	Std 7	2024-04-13 01:04:41 UTC-4	used

Nitrate (Anions)

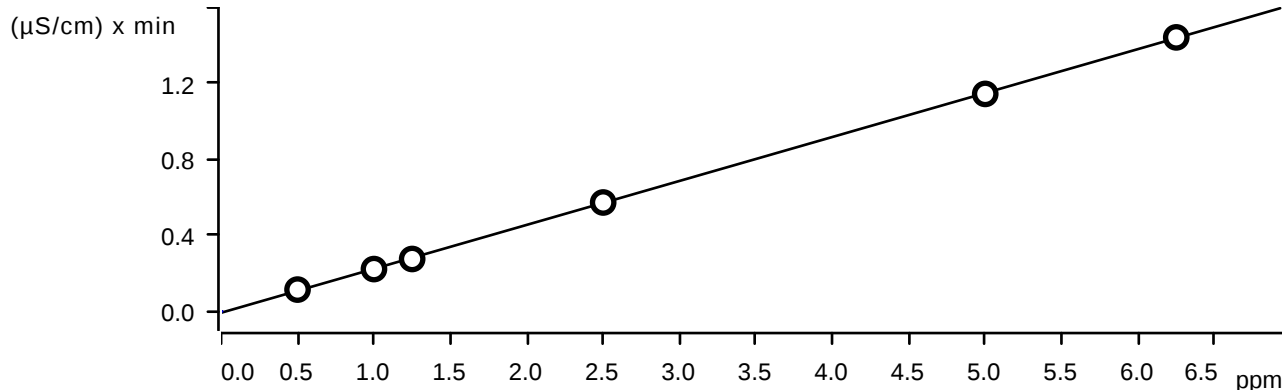


Function: $A = -7.15004E-3 + 0.0231424 \times Q$
 Relative standard deviation: 0.870938 %

Correlation coefficient 0.999960

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.115	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.223	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.276	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.573	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.145	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.443	Std 7	2024-04-13 01:04:41 UTC-4	used

Phosphate (Anions)


(μS/cm) x min

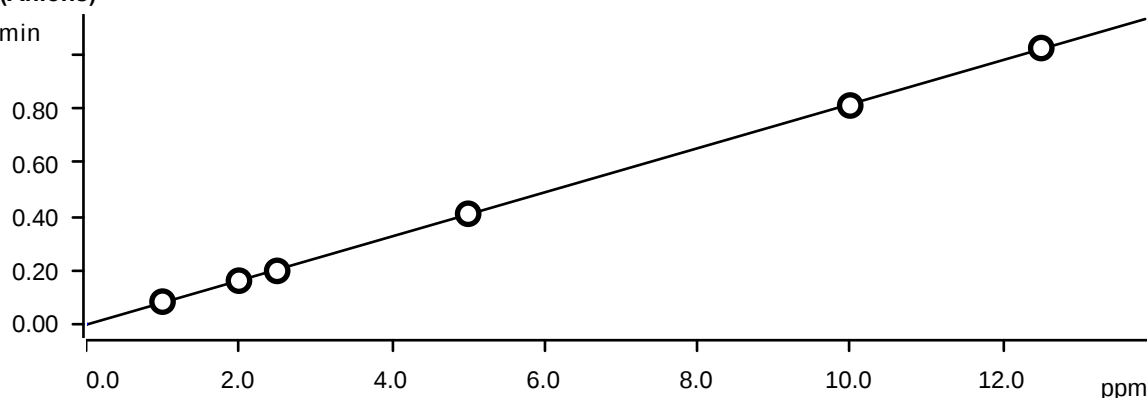Function: $A = -2.37452E-3 + 8.19864E-3 \times Q$

Relative standard deviation 1.011855 %

Correlation coefficient 0.999945

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.083	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.161	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.198	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.410	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.813	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.026	Std 7	2024-04-13 01:04:41 UTC-4	used

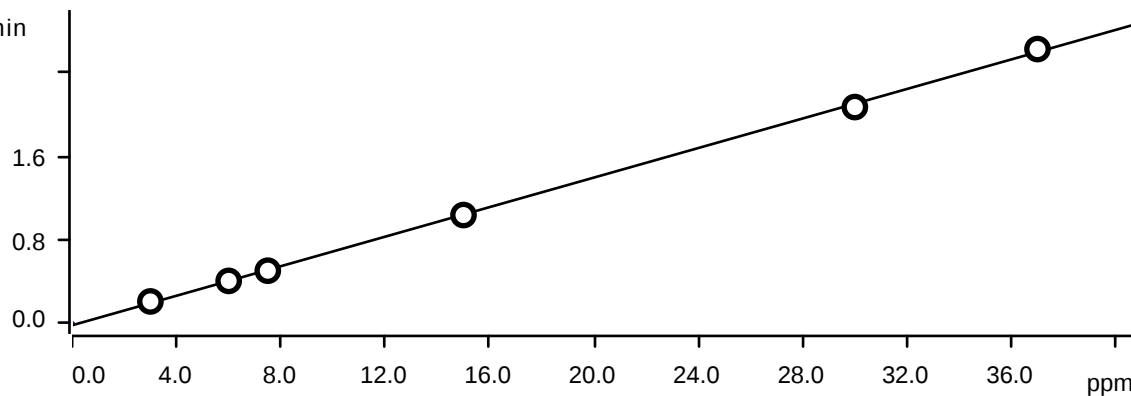Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0233221 + 7.09240E-3 \times Q$

Relative standard deviation 2.047074 %

Correlation coefficient 0.999778

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.206	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.403	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.501	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.035	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.072	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.629	Std 7	2024-04-13 01:04:41 UTC-4	used


Sample data

Ident Std 1
 Sample type Standard 1
 Determination start 2024-04-12 22:45:19 UTC-4
 Method anions
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.32 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

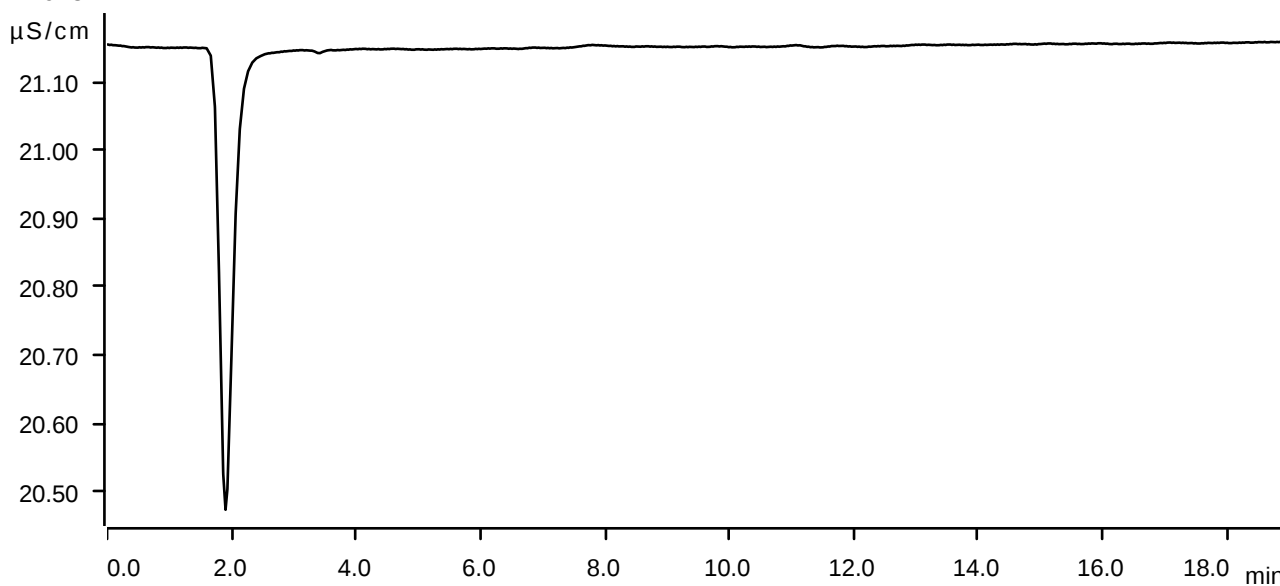


Sample data

Ident Std 2
Sample type Standard 2
Determination start 2024-04-12 23:06:41 UTC-4
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

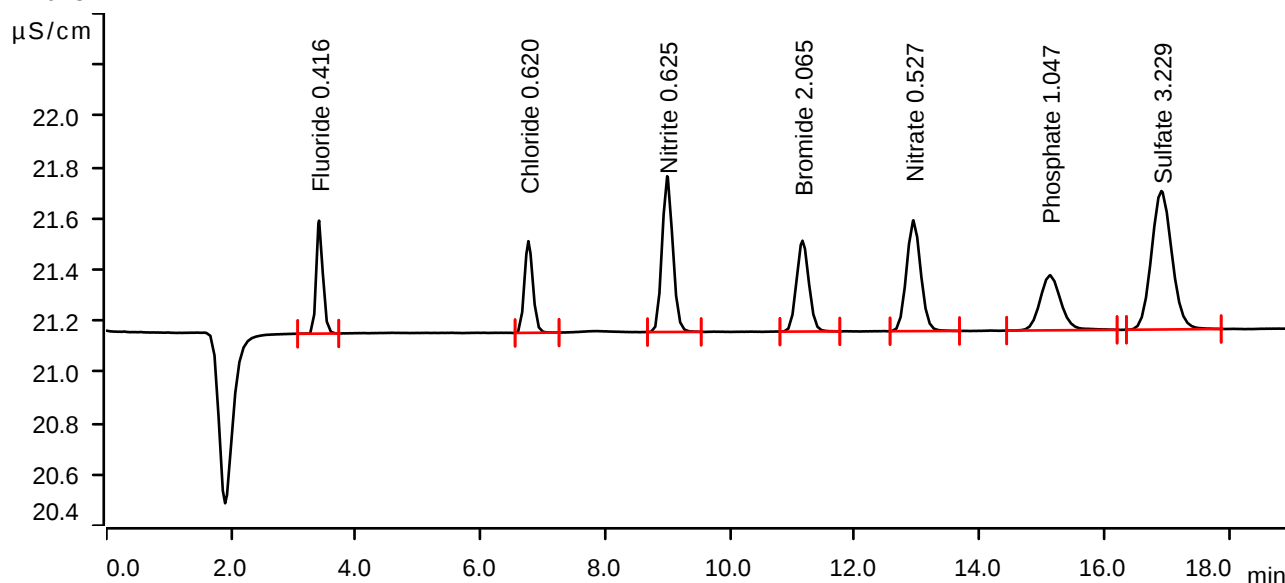

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.412	0.0541	0.441	0.416	Fluoride
2	6.767	0.0561	0.358	0.620	Chloride
3	8.993	0.1216	0.608	0.625	Nitrite
4	11.162	0.0816	0.355	2.065	Bromide
5	12.940	0.1148	0.433	0.527	Nitrate
6	15.127	0.0834	0.215	1.047	Phosphate
7	16.915	0.2057	0.541	3.229	Sulfate


Sample data

Ident Std 3
Sample type Standard 3
Determination start 2024-04-12 22:38:39 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.5 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

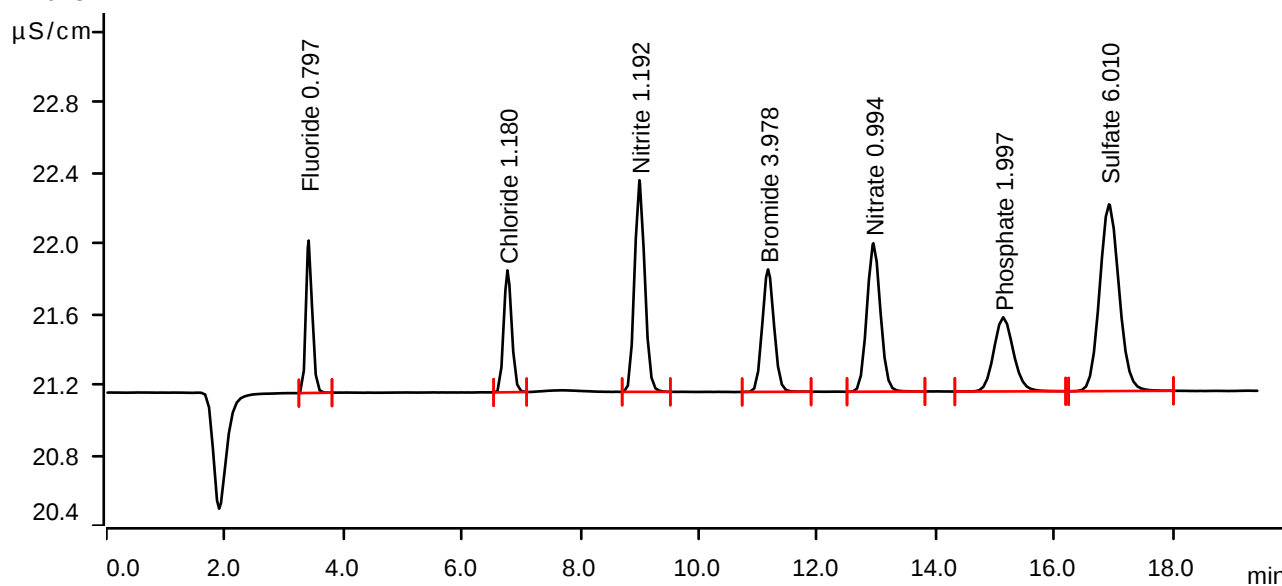

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.415	0.1064	0.863	0.797	Fluoride
2	6.770	0.1076	0.690	1.180	Chloride
3	8.997	0.2391	1.198	1.192	Nitrite
4	11.167	0.1600	0.694	3.978	Bromide
5	12.945	0.2229	0.840	0.994	Nitrate
6	15.137	0.1614	0.420	1.997	Phosphate
7	16.922	0.4029	1.057	6.010	Sulfate


Sample data

Ident Std 4
Sample type Standard 4
Determination start 2024-04-12 23:00:33 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

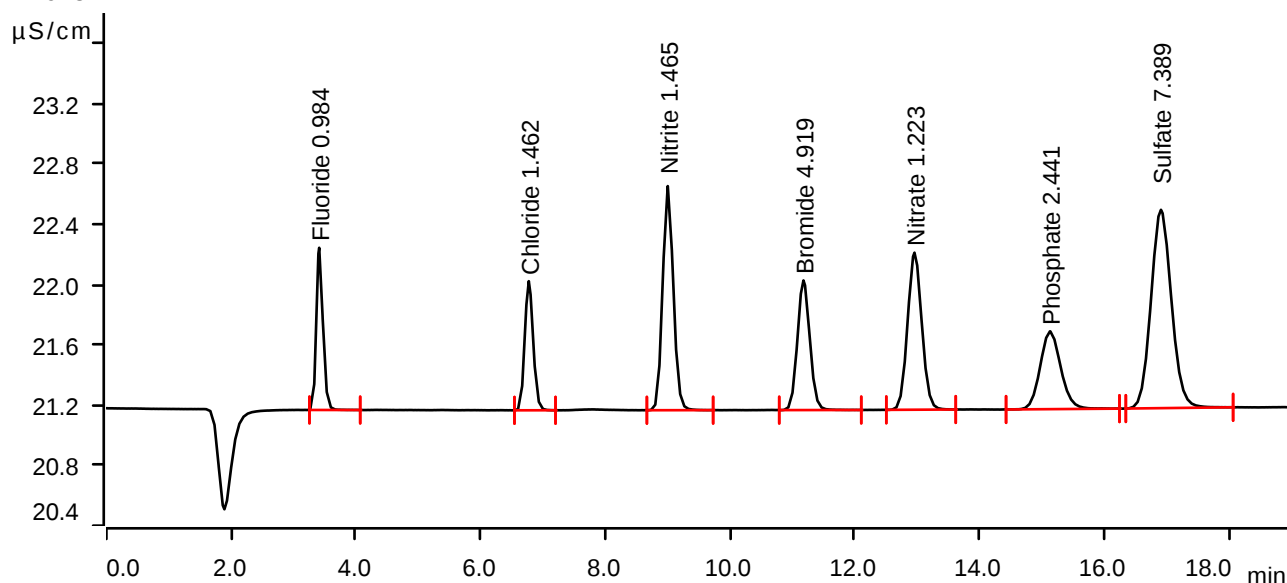

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.413	0.1321	1.077	0.984	Fluoride
2	6.773	0.1336	0.857	1.462	Chloride
3	9.002	0.2959	1.487	1.465	Nitrite
4	11.177	0.1985	0.861	4.919	Bromide
5	12.957	0.2759	1.043	1.223	Nitrate
6	15.128	0.1978	0.517	2.441	Phosphate
7	16.908	0.5007	1.317	7.389	Sulfate


Sample data

Ident Std 5
Sample type Standard 5
Determination start 2024-04-12 23:21:58 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

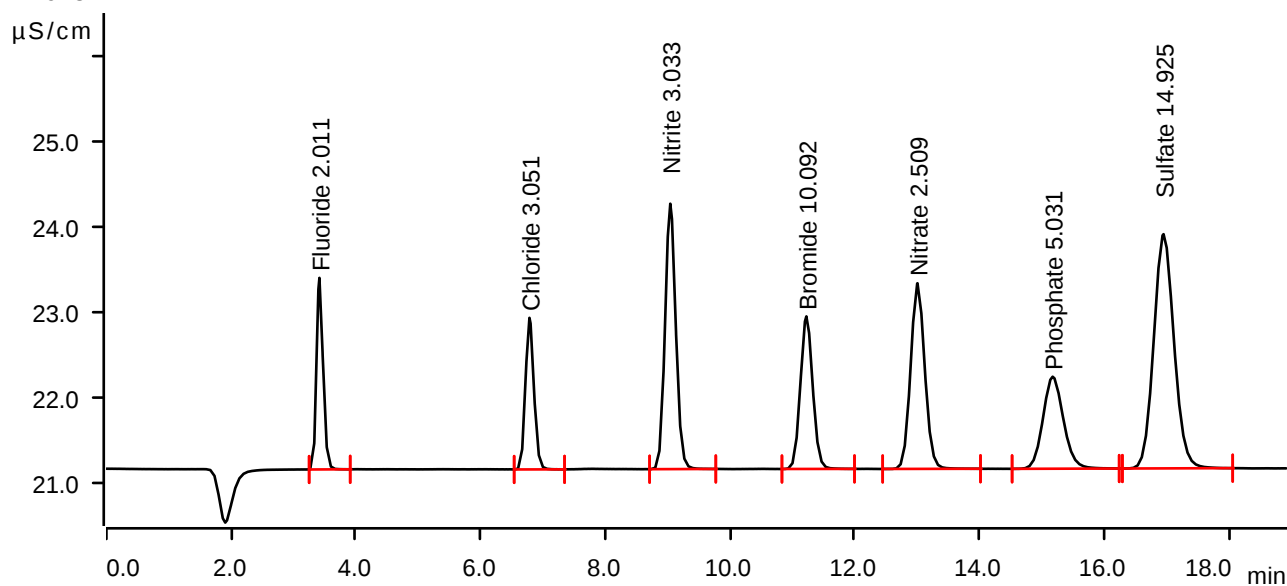

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.417	0.2731	2.244	2.011	Fluoride
2	6.783	0.2800	1.776	3.051	Chloride
3	9.042	0.6213	3.109	3.033	Nitrite
4	11.223	0.4104	1.788	10.092	Bromide
5	13.005	0.5735	2.175	2.509	Nitrate
6	15.172	0.4101	1.078	5.031	Phosphate
7	16.950	1.0352	2.744	14.925	Sulfate


Sample data

Ident Std 6
Sample type Standard 6
Determination start 2024-04-12 23:43:14 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

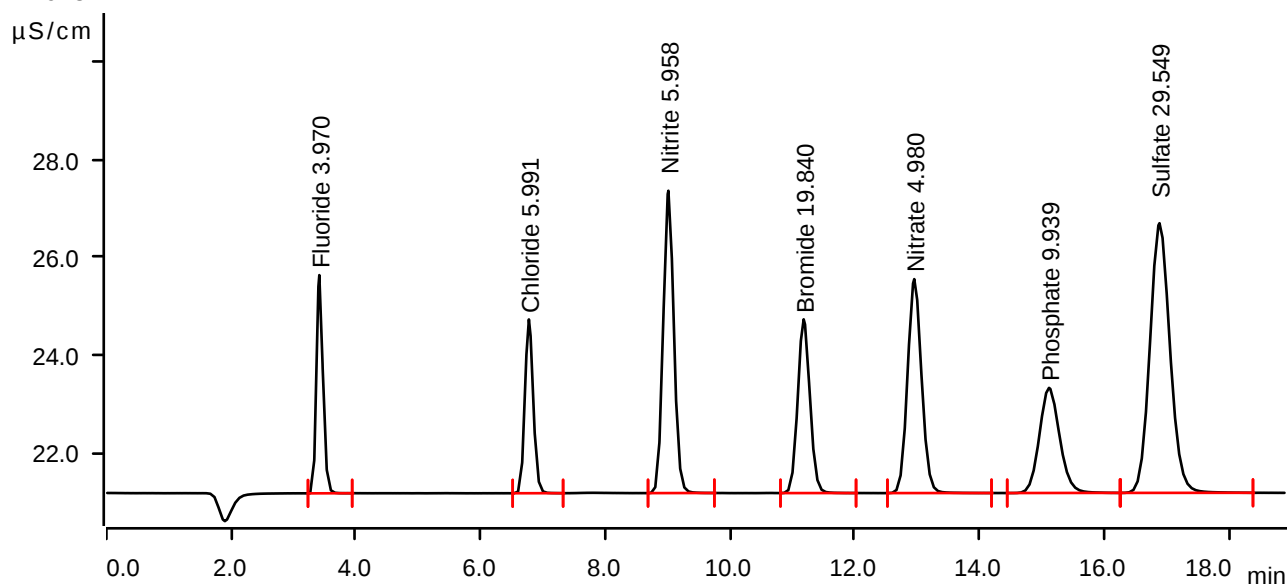

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.415	0.5422	4.473	3.970	Fluoride
2	6.775	0.5509	3.563	5.991	Chloride
3	9.012	1.2283	6.198	5.958	Nitrite
4	11.180	0.8095	3.562	19.840	Bromide
5	12.953	1.1453	4.386	4.980	Nitrate
6	15.113	0.8125	2.155	9.939	Phosphate
7	16.885	2.0724	5.528	29.549	Sulfate


Sample data

Ident Std 7
Sample type Standard 7
Determination start 2024-04-13 00:04:41 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

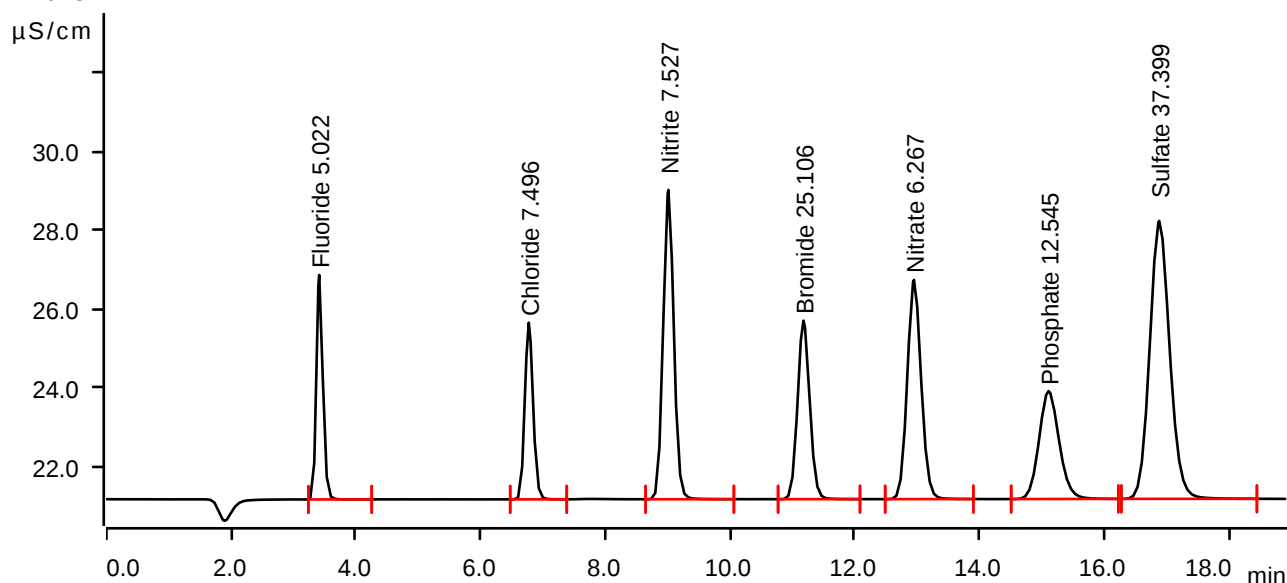

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.413	0.6867	5.697	5.022	Fluoride
2	6.773	0.6894	4.484	7.496	Chloride
3	9.012	1.5538	7.851	7.527	Nitrite
4	11.177	1.0252	4.531	25.106	Bromide
5	12.948	1.4431	5.565	6.267	Nitrate
6	15.107	1.0261	2.739	12.545	Phosphate
7	16.880	2.6292	7.053	37.399	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2024-04-13 02:35:03 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

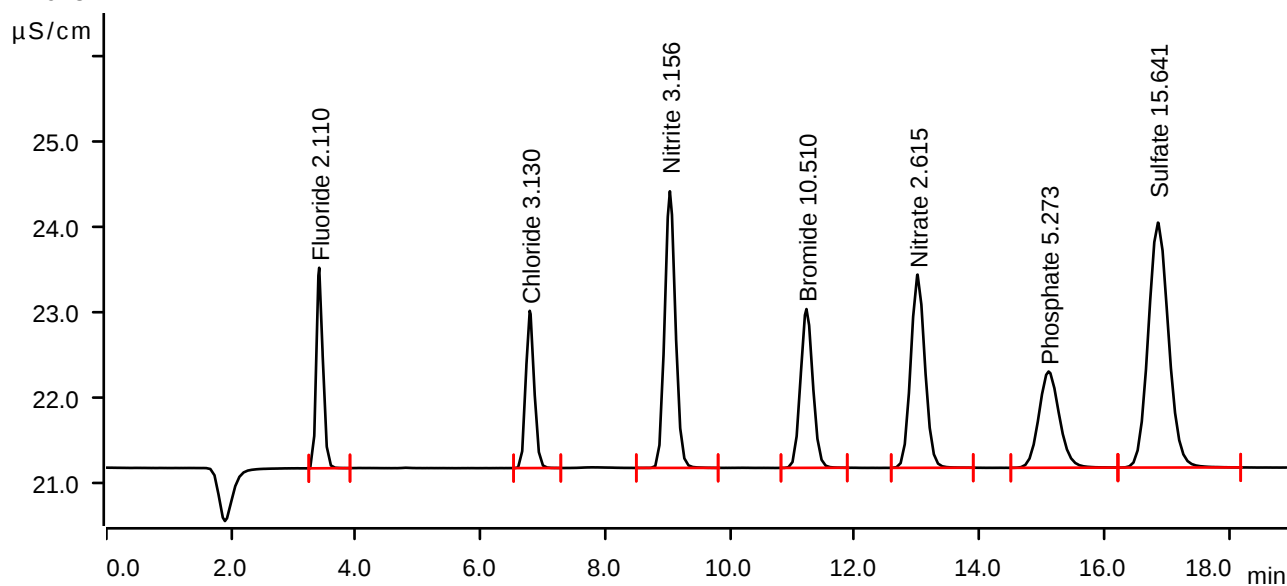


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.413	0.2867	2.349	2.110	Fluoride
2	6.788	0.2873	1.842	3.130	Chloride
3	9.035	0.6468	3.241	3.156	Nitrite
4	11.225	0.4275	1.860	10.510	Bromide
5	13.007	0.5980	2.263	2.615	Nitrate
6	15.107	0.4300	1.127	5.273	Phosphate
7	16.860	1.0860	2.869	15.641	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2024-04-13 02:56:34 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

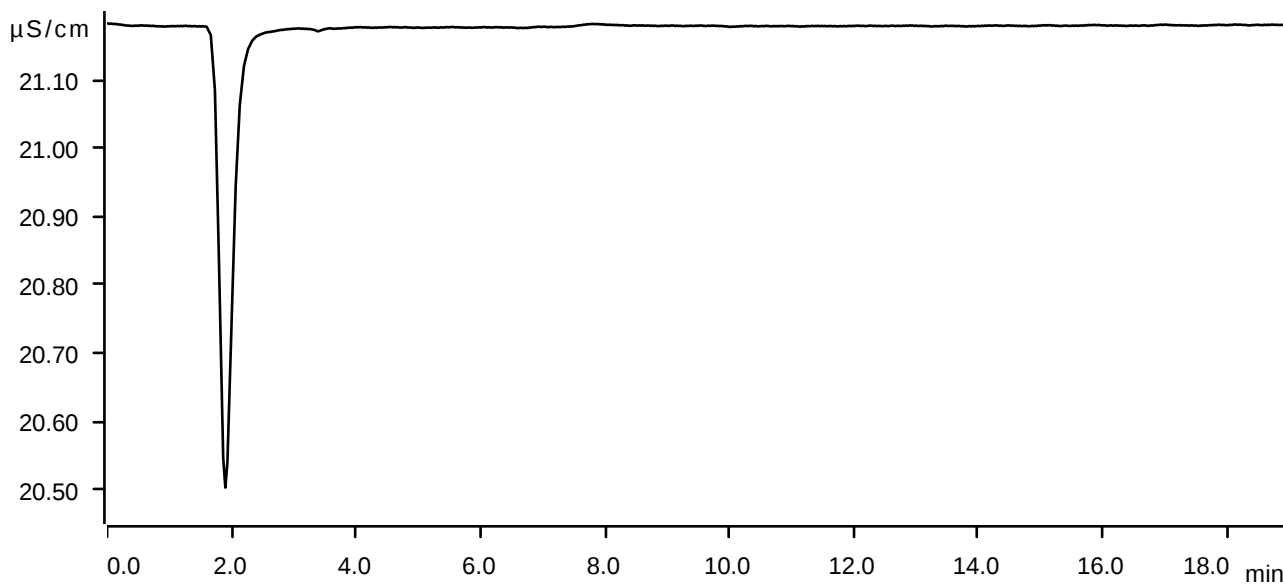Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-05-23 09:44:28 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

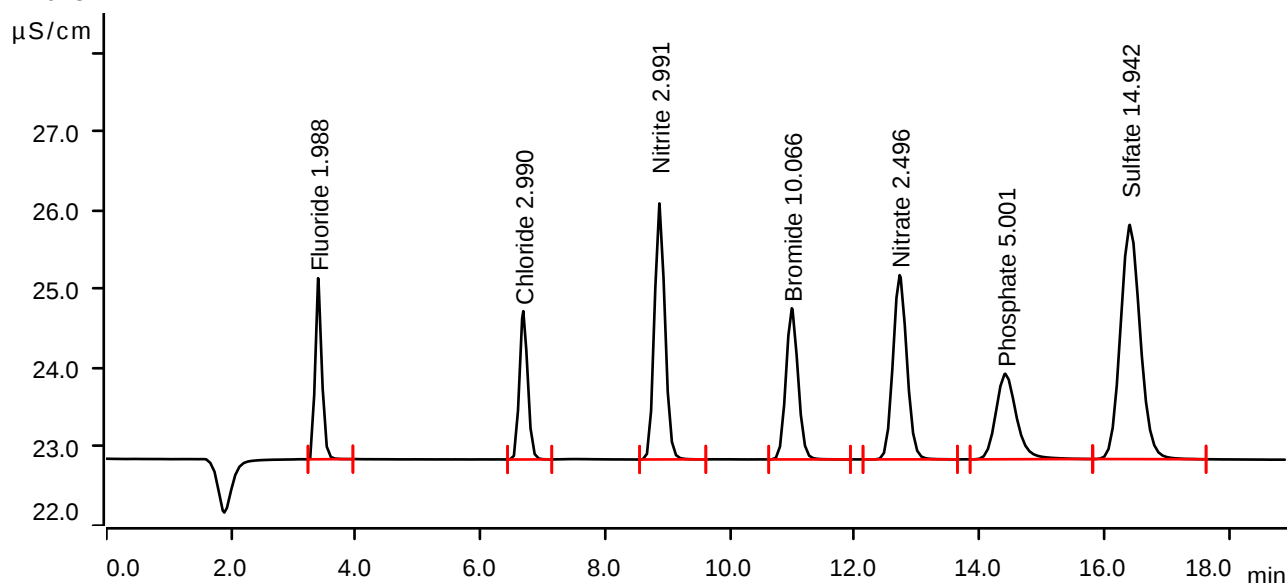


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.2838	2.298	1.988	Fluoride
2	6.685	0.2892	1.882	2.990	Chloride
3	8.868	0.6372	3.249	2.991	Nitrite
4	10.990	0.4329	1.918	10.066	Bromide
5	12.718	0.6047	2.338	2.496	Nitrate
6	14.413	0.4161	1.085	5.001	Phosphate
7	16.408	1.0946	2.973	14.942	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-05-23 10:05:58 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

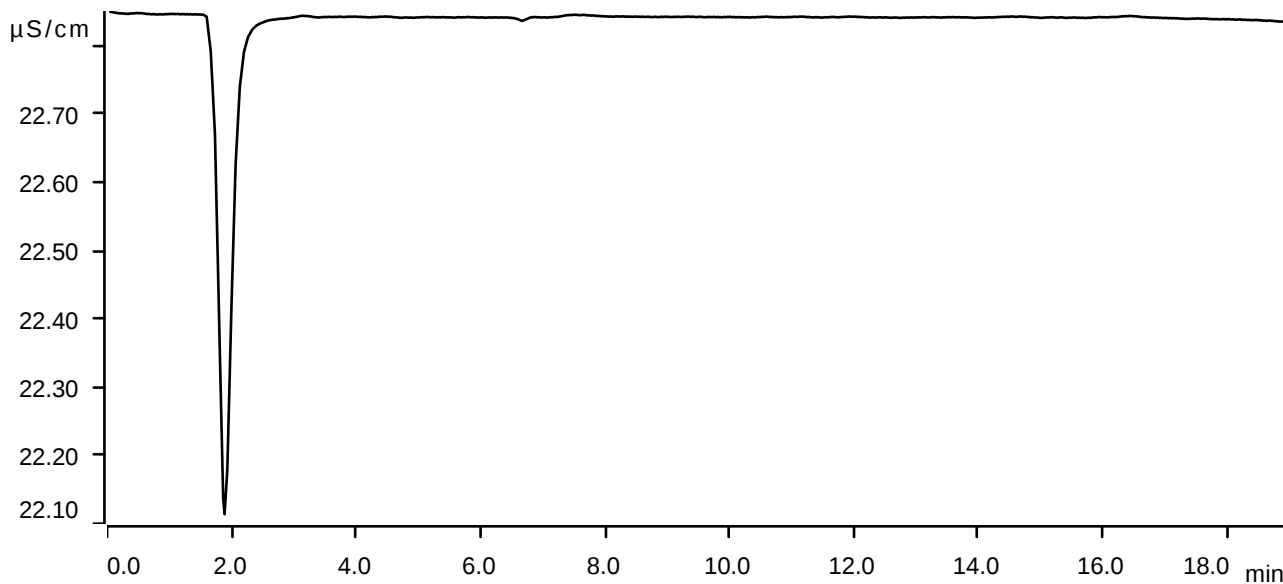Anions


Sample data

Ident LB130917BLW
Sample type Sample
Determination start 2024-05-23 10:27:28 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

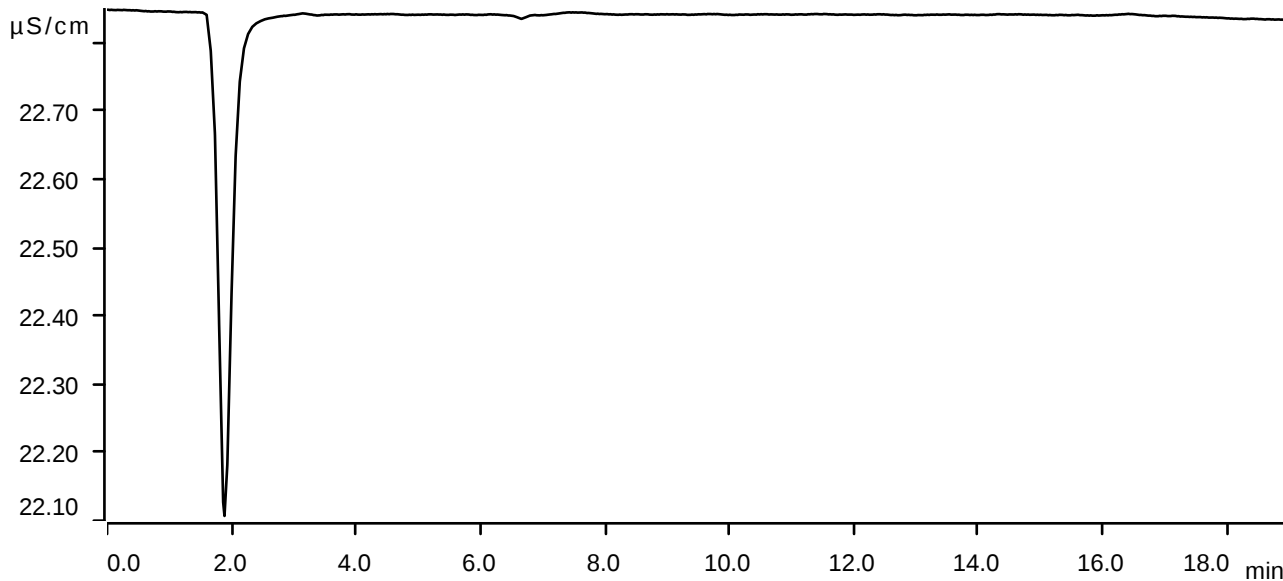


Sample data

Ident LB130917BSW
Sample type Check standard 1
Determination start 2024-05-23 10:48:58 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

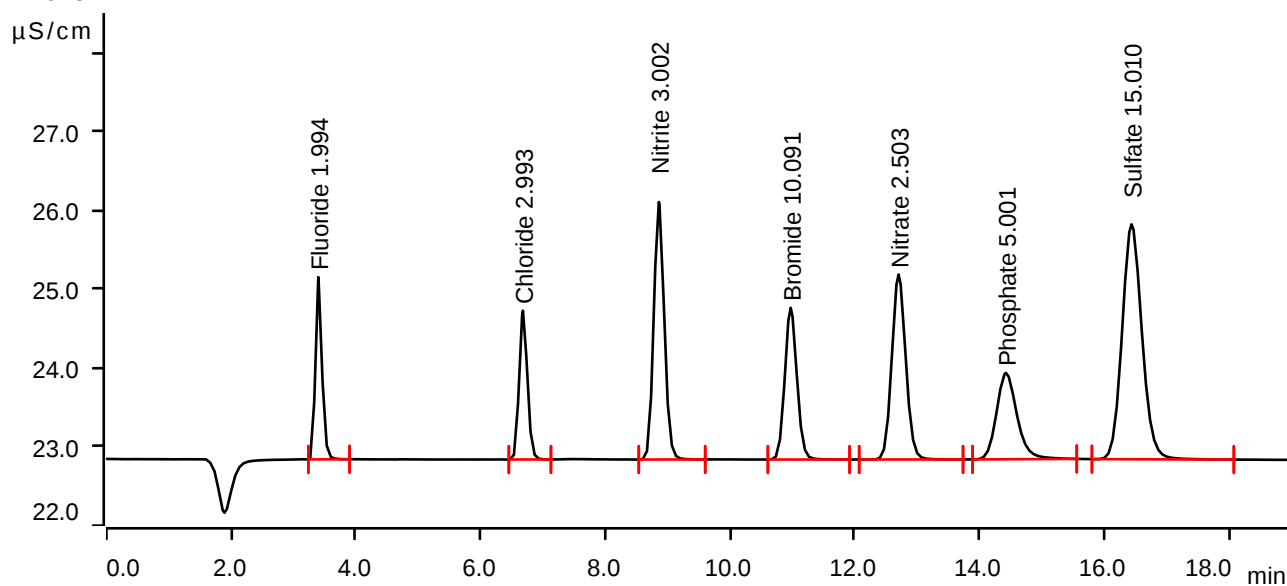

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.398	0.2847	2.313	1.994	Fluoride
2	6.680	0.2896	1.888	2.993	Chloride
3	8.858	0.6398	3.267	3.002	Nitrite
4	10.972	0.4339	1.926	10.091	Bromide
5	12.702	0.6066	2.347	2.503	Nitrate
6	14.423	0.4161	1.096	5.001	Phosphate
7	16.437	1.0997	2.981	15.010	Sulfate


Sample data

Ident P2582-01
Sample type Sample
Determination start 2024-05-23 11:10:30 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

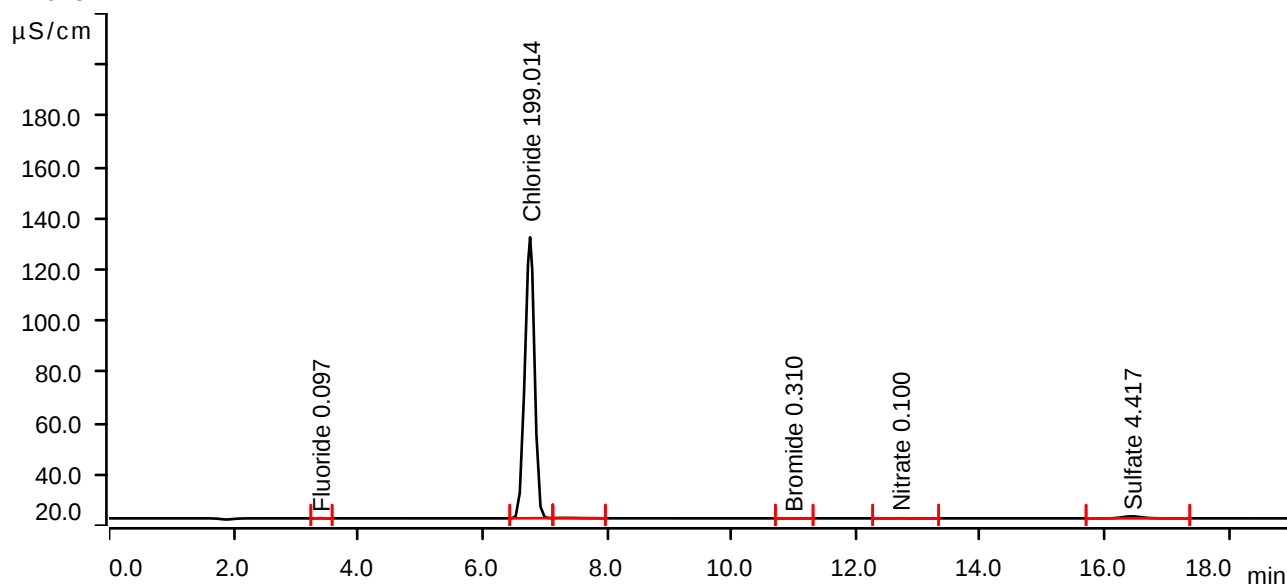

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.0085	0.070	0.097	Fluoride
2	6.767	19.5703	109.703	199.014	Chloride
3	7.340	0.0266	0.071	invalid	
4	10.982	0.0036	0.016	0.310	Bromide
5	12.705	0.0111	0.042	0.100	Nitrate
6	16.432	0.2955	0.797	4.417	Sulfate


Sample data

Ident P2582-01MS
Sample type Sample
Determination start 2024-05-23 11:32:02 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

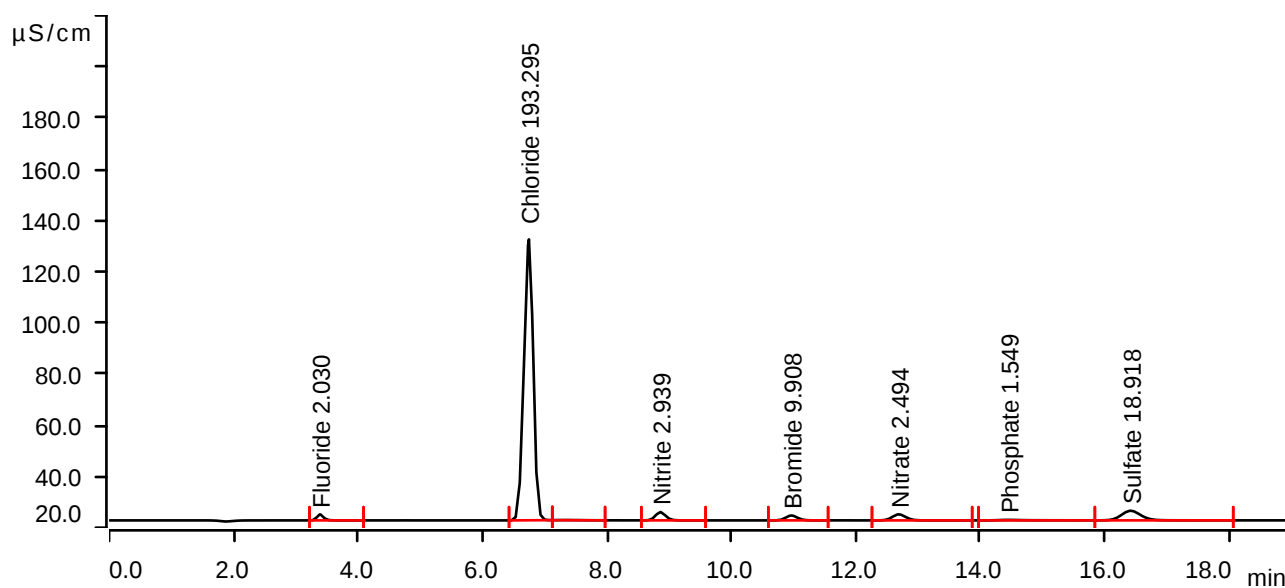

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.387	0.2899	2.357	2.030	Fluoride
2	6.748	19.0078	109.683	193.295	Chloride
3	7.338	0.0243	0.064	invalid	
4	8.860	0.6259	3.245	2.939	Nitrite
5	10.965	0.4259	1.915	9.908	Bromide
6	12.690	0.6043	2.355	2.494	Nitrate
7	14.455	0.1212	0.194	1.549	Phosphate
8	16.417	1.3964	3.765	18.918	Sulfate


Sample data

Ident P2582-01MSD
Sample type Sample
Determination start 2024-05-23 11:53:36 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

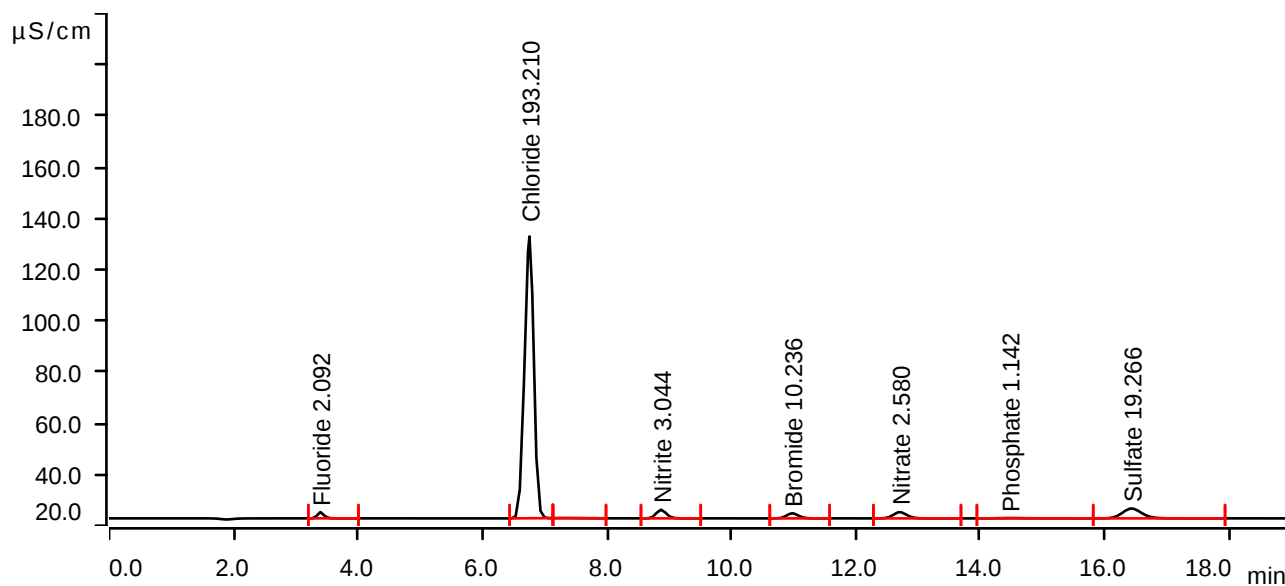

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.2990	2.417	2.092	Fluoride
2	6.757	18.9994	110.034	193.210	Chloride
3	7.352	0.0236	0.063	invalid	
4	8.870	0.6490	3.363	3.044	Nitrite
5	10.978	0.4403	1.977	10.236	Bromide
6	12.707	0.6256	2.434	2.580	Nitrate
7	14.472	0.0864	0.140	1.142	Phosphate
8	16.430	1.4229	3.854	19.266	Sulfate


Sample data

Ident P2582-01DLX50
Sample type Sample
Determination start 2024-05-23 12:15:09 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

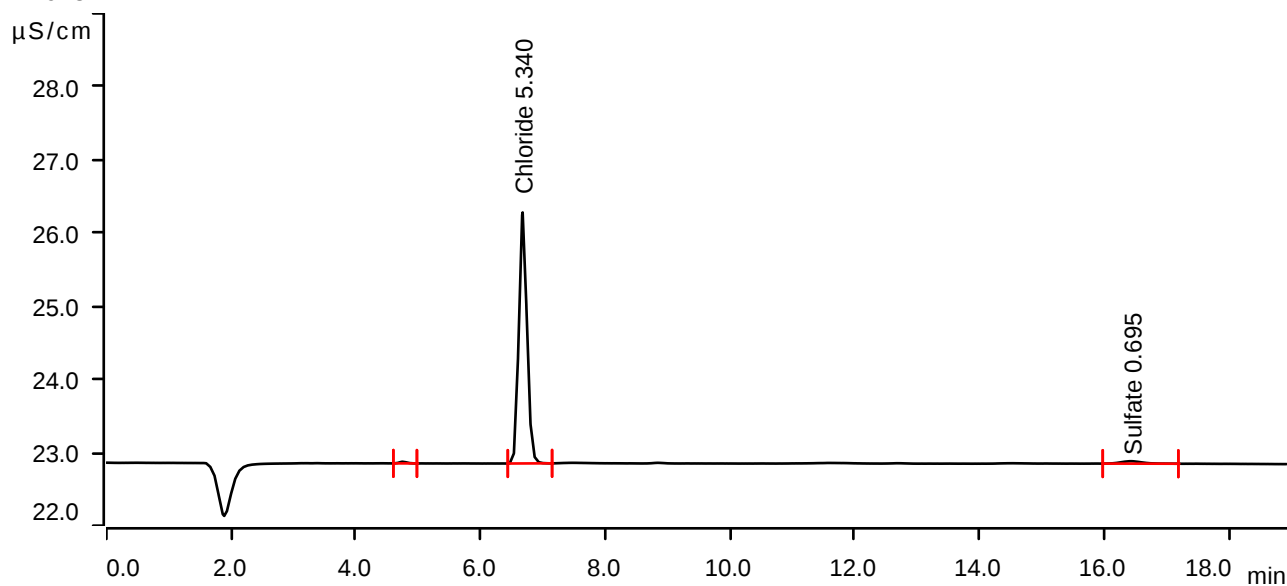

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	4.748	0.0032	0.022	invalid	
2	6.675	0.5204	3.430	5.340	Chloride
3	16.410	0.0129	0.033	0.695	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-05-23 12:36:44 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

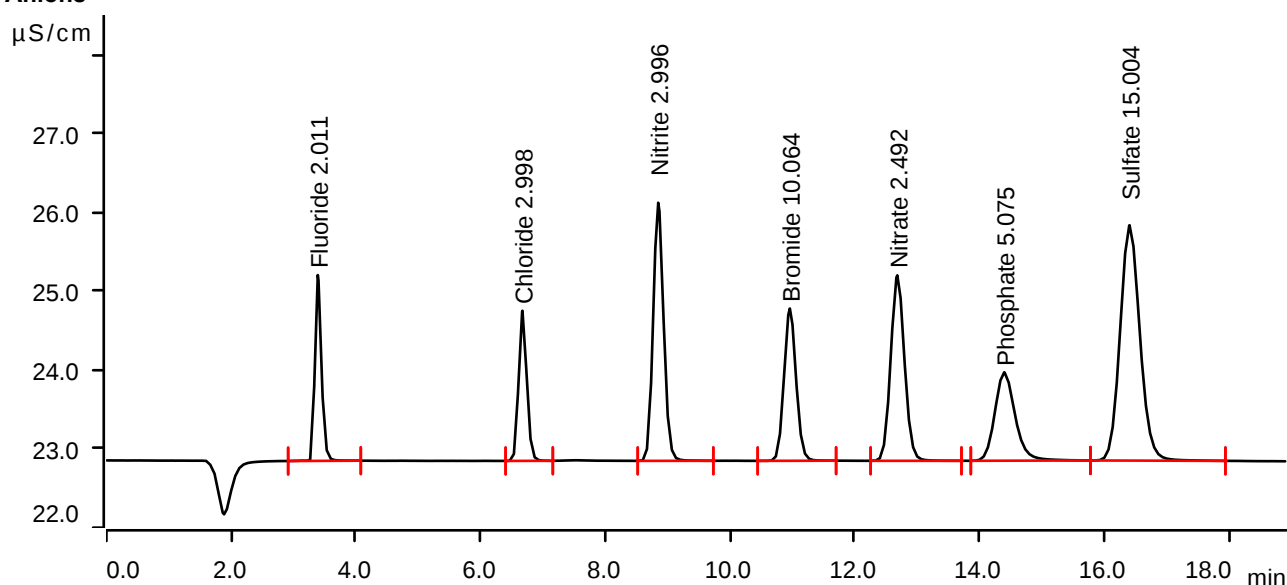


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.2871	2.358	2.011	Fluoride
2	6.672	0.2900	1.905	2.998	Chloride
3	8.848	0.6385	3.275	2.996	Nitrite
4	10.958	0.4328	1.933	10.064	Bromide
5	12.682	0.6039	2.354	2.492	Nitrate
6	14.395	0.4224	1.121	5.075	Phosphate
7	16.405	1.0993	2.987	15.004	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-05-23 12:58:13 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

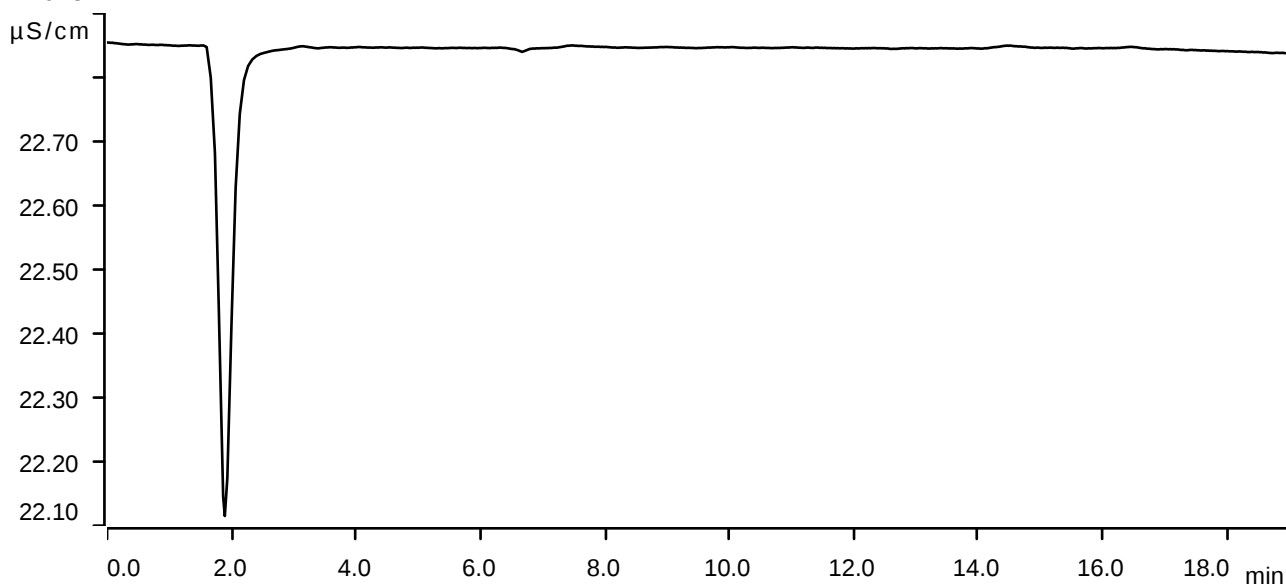Anions

WORKLIST(Hardcopy Internal Chain)

LB130917

WorkList Name : ANINONS-05232024

WorkList ID : 180521

Department : Wet-Chemistry

Date : 05-23-2024 09:59:38

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P2582-01	SY-3	Water	Anions Group1	Cool 4 deg C	LOCK01	K21	05/22/2024	300.0

Date/Time 05.23.2024, 10:30
Raw Sample Received by: NF(wc)
Raw Sample Relinquished by: JF Collier

Date/Time 05.23.2024, 11:15
Raw Sample Received by: M Cole
Raw Sample Relinquished by: NF(wc)