


LB130934

7471B

INSTRUMENT ID: CY1

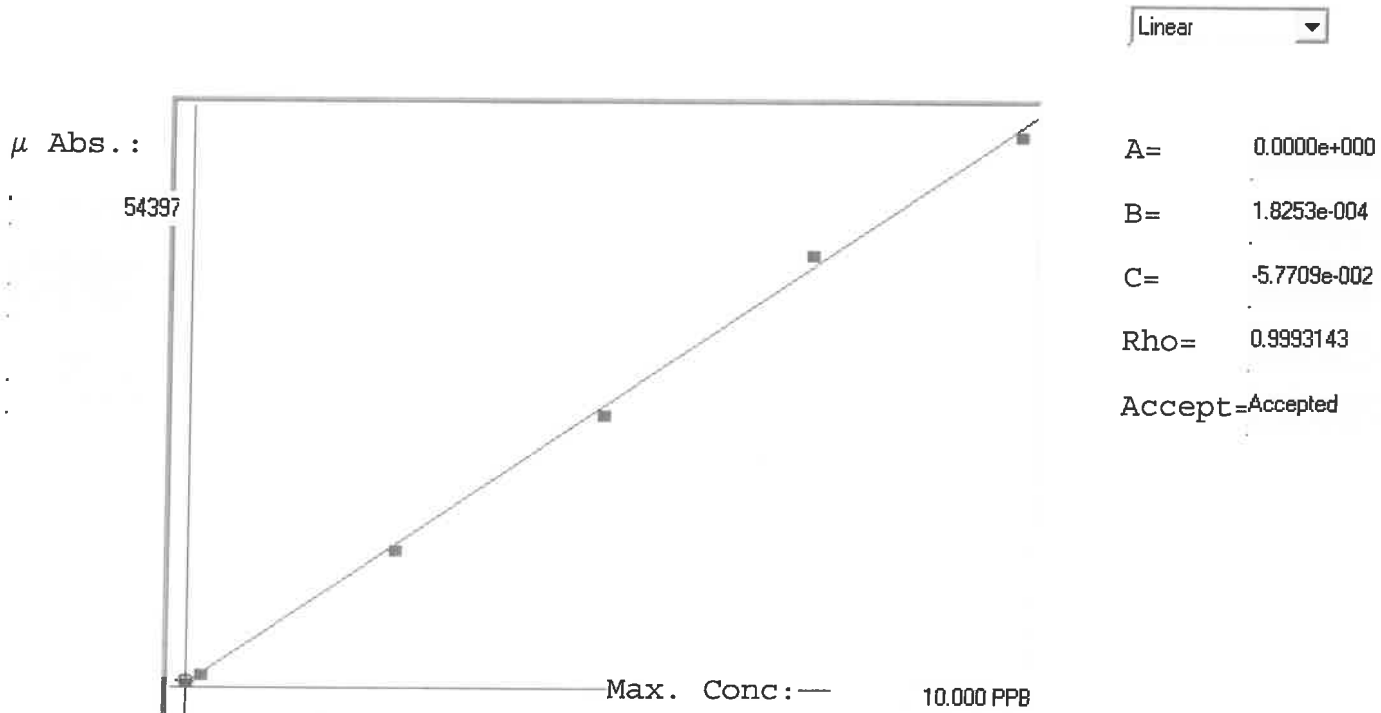

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%1)
0.0	0.000	0.061	0.061	653	0.000	653					-
0.2	0.200	0.193	-0.007	1374	0.0 %	1374					-4
2.5	2.500	2.443	-0.057	13699	0.0 %	13699					-2
5.0	5.000	4.866	-0.134	26977	0.0 %	26977					-3
7.5	7.500	7.765	0.265	42860	0.0 %	42860					4
10.0	10.000	9.871	-0.129	54397	0.0 %	54397					-1

LB130934 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 29 May 2024 11:13:34

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	653	-	0.0000	7471B	PPB	29 May 2024 11:14:49	S	Std
0.2 - 1	51.2	1374	-	0.2000	7471B	PPB	29 May 2024 11:17:06	S	Std
2.5 - 1	52.5	13699	-	2.5000	7471B	PPB	29 May 2024 11:19:23	S	Std
5.0 - 1	55	26977	-	5.0000	7471B	PPB	29 May 2024 11:21:41	S	Std
7.5 - 1	57.5	42860	-	7.5000	7471B	PPB	29 May 2024 11:24:00	S	Std
10.0 - 1	514	54397	-	10.0000	7471B	PPB	29 May 2024 11:26:18	S	Std
ICV65 - 1	ICV65	21789	3.9193	-	7471B	PPB	29 May 2024 11:29:11	U	SMPL
ICB65 - 1	ICB65	104	-0.0387	-	7471B	PPB	29 May 2024 11:31:27	U	SMPL
CCV50 - 1	CCV50	28311	5.1098	-	7471B	PPB	29 May 2024 11:33:45	U	SMPL
CCB50 - 1	CCB50	78	-0.0435	-	7471B	PPB	29 May 2024 11:36:00	U	SMPL
CRA - 1	CRA	1463	0.2093	-	7471B	PPB	29 May 2024 11:38:19	U	SMPL
HighStd - 1	HighStd	54848	9.9534	-	7471B	PPB	29 May 2024 11:40:35	U	SMPL
ChkStd - 1	ChkStd	39747	7.1971	-	7471B	PPB	29 May 2024 11:42:50	U	SMPL
PB161124BL - 1	PBS	-231	-0.0999	-	7471B	PPB	29 May 2024 11:45:15	U	SMPL
PB161124BS - 1	LCSS	19734	3.5442	-	7471B	PPB	29 May 2024 11:50:12	U	SMPL
P2578-01 - 1	OR-02-052224	4809	0.8201	-	7471B	PPB	29 May 2024 11:57:31	U	SMPL
P2578-01DUP - 1	OR-02-052224DUP	4916	0.8396	-	7471B	PPB	29 May 2024 11:59:47	U	SMPL
P2578-01MS - 1	OR-02-052224MS	25391	4.5768	-	7471B	PPB	29 May 2024 12:02:06	U	SMPL
P2578-01MSD - 1	OR-02-052224MSD	24667	4.4446	-	7471B	PPB	29 May 2024 12:07:26	U	SMPL
P2580-01 - 1	TR-05-052224	1916	0.2920	-	7471B	PPB	29 May 2024 12:09:40	U	SMPL
CCV51 - 1	CCV51	27640	4.9873	-	7471B	PPB	29 May 2024 12:11:58	U	SMPL
CCB51 - 1	CCB51	-49	-0.0667	-	7471B	PPB	29 May 2024 12:14:14	U	SMPL
P2597-01 - 1	PL-01-052324	1919	0.2926	-	7471B	PPB	29 May 2024 12:16:32	U	SMPL
P2611-01 - 1	AU-06-052424	1572	0.2292	-	7471B	PPB	29 May 2024 12:18:47	U	SMPL
P2612-01 - 1	VNJ-203	13683	2.4398	-	7471B	PPB	29 May 2024 12:21:04	U	SMPL
P2612-04 - 1	RT1486	7461	1.3041	-	7471B	PPB	29 May 2024 12:23:20	U	SMPL
P2612-07 - 1	RBR200057	13750	2.4520	-	7471B	PPB	29 May 2024 12:25:39	U	SMPL
P2612-10 - 1	72-11933	12311	2.1894	-	7471B	PPB	29 May 2024 12:27:57	U	SMPL
P2613-01 - 1	TR-06-052424	1299	0.1794	-	7471B	PPB	29 May 2024 12:30:16	U	SMPL
P2615-01 - 1	RBR251686	21935	3.9460	-	7471B	PPB	29 May 2024 12:32:35	U	SMPL
P2615-03 - 1	RBR200035	3204	0.5271	-	7471B	PPB	29 May 2024 12:34:52	U	SMPL
P2616-01 - 1	VNJ-206	3580	0.5957	-	7471B	PPB	29 May 2024 12:37:10	U	SMPL
CCV52 - 1	CCV52	27727	5.0032	-	7471B	PPB	29 May 2024 12:39:27	U	SMPL
CCB52 - 1	CCB52	36	-0.0511	-	7471B	PPB	29 May 2024 12:41:43	U	SMPL
P2578-01LX5 - 1		1026	0.1296	-	7471B	PPB	29 May 2024 12:44:02	U	SMPL
P2578-01A - 1		25235	4.5483	-	7471B	PPB	29 May 2024 12:46:18	U	SMPL
CCV53 - 1	CCV53	28425	5.1306	-	7471B	PPB	29 May 2024 12:48:34	U	SMPL
CCB53 - 1	CCB53	250	-0.0121	-	7471B	PPB	29 May 2024 12:50:52	U	SMPL