


LB130986

7470A

INSTRUMENT ID: CV1

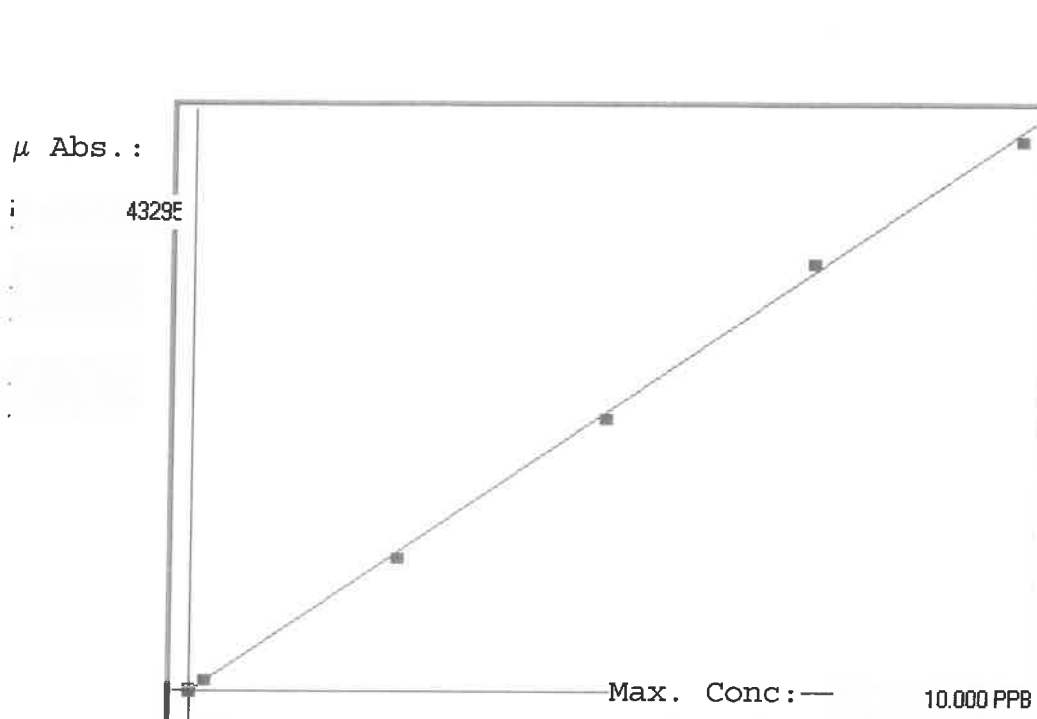

Linear

A= 0.0000e+000

B= 2.2780e-004

C= 2.5152e-002

Rho= 0.9996055

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/p
0.0	0.000	0.006	0.006	-85	0.000	-85	0				-
0.2	0.200	0.238	0.038	933	0.0 %	933					19
2.5	2.500	2.420	-0.080	10514	0.0 %	10514					-3
5.0	5.000	4.946	-0.054	21600	0.0 %	21600					-1
7.5	7.500	7.703	0.203	33703	0.0 %	33703					3
10.0	10.000	9.888	-0.112	43295	0.0 %	43295					-1

LB130986 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 30 May 2024 11:24:13

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-85	-	0.0000	7470A	PPB	30 May 2024 11:41:58	S	Std
0.2 - 1	50-2	933	-	0.2000	7470A	PPB	30 May 2024 11:44:15	S	Std
2.5 - 1	52-5	10514	-	2.5000	7470A	PPB	30 May 2024 11:46:32	S	Std
5.0 - 1	55	21600	-	5.0000	7470A	PPB	30 May 2024 11:48:49	S	Std
7.5 - 1	57-5	33703	-	7.5000	7470A	PPB	30 May 2024 11:51:07	S	Std
10.0 - 1	510	43295	-	10.0000	7470A	PPB	30 May 2024 12:01:47	S	Std
ICV67 - 1	ICV67	18199	4.1709	-	7470A	PPB	30 May 2024 12:09:14	U	SMPL
ICB67 - 1	ICB67	-128	-0.0040	-	7470A	PPB	30 May 2024 12:11:32	U	SMPL
CCV58 - 1	CCV58	20402	4.6728	-	7470A	PPB	30 May 2024 12:13:49	U	SMPL
CCB58 - 1	CCB58	-131	-0.0047	-	7470A	PPB	30 May 2024 12:16:04	U	SMPL
CRA - 1	CRA	892	0.2284	-	7470A	PPB	30 May 2024 12:18:21	U	SMPL
HighStd - 1	HighStd	42670	9.7455	-	7470A	PPB	30 May 2024 12:20:36	U	SMPL
ChkStd - 1	ChkStd	31139	7.1187	-	7470A	PPB	30 May 2024 12:22:51	U	SMPL
PB161185BL - 1	PBW	-318	-0.0473	-	7470A	PPB	30 May 2024 12:25:10	U	SMPL
PB161185BS - 1	LCSW	16402	3.7616	-	7470A	PPB	30 May 2024 12:27:29	U	SMPL
P2612-03 - 1	VNJ-203	-156	-0.0104	-	7470A	PPB	30 May 2024 12:29:46	U	SMPL
P2612-06 - 1	RT1486	45	0.0354	-	7470A	PPB	30 May 2024 12:32:05	U	SMPL
P2612-09 - 1	RBR200057	104	0.0488	-	7470A	PPB	30 May 2024 12:34:22	U	SMPL
P2612-12 - 1	72-11933	148	0.0589	-	7470A	PPB	30 May 2024 12:36:39	U	SMPL
P2637-04 - 1	WCS-TPT	157	0.0609	-	7470A	PPB	30 May 2024 12:38:55	U	SMPL
CCV59 - 1	CCV59	23048	5.2755	-	7470A	PPB	30 May 2024 12:41:10	U	SMPL
CCB59 - 1	CCB59	-226	-0.0263	-	7470A	PPB	30 May 2024 12:43:25	U	SMPL
P2637-04DUP - 1	WCS-TPTDUP	100	0.0479	-	7470A	PPB	30 May 2024 12:45:43	U	SMPL
P2637-04MS - 1	WCS-TPTMS	17228	3.9497	-	7470A	PPB	30 May 2024 12:50:30	U	SMPL
P2637-04MSD - 1	WCS-TPTMSD	16773	3.8461	-	7470A	PPB	30 May 2024 12:52:48	U	SMPL
PB161142TB - 1		-400	-0.0660	-	7470A	PPB	30 May 2024 12:55:04	U	SMPL
P2637-04LX5 - 1		87	0.0450	-	7470A	PPB	30 May 2024 12:57:23	U	SMPL
P2637-04A - 1		19551	4.4789	-	7470A	PPB	30 May 2024 12:59:40	U	SMPL
CCV60 - 1	CCV60	23205	5.3113	-	7470A	PPB	30 May 2024 13:01:56	U	SMPL
CCB60 - 1	CCB60	-83	0.0062	-	7470A	PPB	30 May 2024 13:06:51	U	SMPL