

66130994

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

5/30/2024 14:29

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.024	0.0	0.109	
ICB1	-0.003	0.0	0.005	
CCV1	1.048	0.0	0.112	
CCB1	-0.001	0.0	0.005	
PB161201BL	-0.001	0.0	0.005	
PB161201BS	1.022	0.0	0.109	
P2403-03	0.027	0.0	0.008	
PB161202BL	0.001	0.0	0.005	
PB161202BS	1.017	0.0	0.108	
P2403-09	0.028	0.0	0.008	
CCV2	1.040	0.0	0.111	
CCB2	0.001	0.0	0.005	

N	12
Mean	0.434
SD	0.5270
CV%	121.54

Aquakem v. 7.2AQ1

Results from time period:

Thu May 30 13:14:04 2024

Thu May 30 14:25:50 2024

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0.0006	mg/l	5/30/2024 13:14:04	
0.05PPM	A	Phenolics-	P	0.0528	mg/l	5/30/2024 13:14:05	
0.1PPM	A	Phenolics-	P	0.1067	mg/l	5/30/2024 13:14:06	
0.25PPM	A	Phenolics-	P	0.262	mg/l	5/30/2024 13:14:07	
0.50PPM	A	Phenolics-	P	0.4967	mg/l	5/30/2024 13:14:08	
1.0PPM	A	Phenolics-	P	0.9644	mg/l	5/30/2024 13:14:09	
2.0PPM	A	Phenolics-	P	2.0167	mg/l	5/30/2024 13:14:10	
ICV1	S	Phenolics-	P	1.0238	mg/l	5/30/2024 14:13:04	
ICB1	S	Phenolics-	P	-0.0029	mg/l	5/30/2024 14:13:06	
CCV1	S	Phenolics-	P	1.0482	mg/l	5/30/2024 14:13:07	
CCB1	S	Phenolics-	P	-0.0014	mg/l	5/30/2024 14:13:09	
PB161201BL	S	Phenolics-	P	-0.001	mg/l	5/30/2024 14:13:12	
PB161201BS	S	Phenolics-	P	1.0224	mg/l	5/30/2024 14:13:13	
P2403-03	S	Phenolics-	P	0.0272	mg/l	5/30/2024 14:23:02	
PB161202BL	S	Phenolics-	P	0.0008	mg/l	5/30/2024 14:23:05	
PB161202BS	S	Phenolics-	P	1.0173	mg/l	5/30/2024 14:23:08	
P2403-09	S	Phenolics-	P	0.0277	mg/l	5/30/2024 14:23:09	
CCV2	S	Phenolics-	P	1.0402	mg/l	5/30/2024 14:23:11	
CCB2	S	Phenolics-	P	0.0008	mg/l	5/30/2024 14:23:13	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

5/30/2024 13:46


Test Phenolics-

Accepted 5/30/2024 13:45

Factor 9.837
Bias 0.005

Coeff. of det. 0.999444

Errors

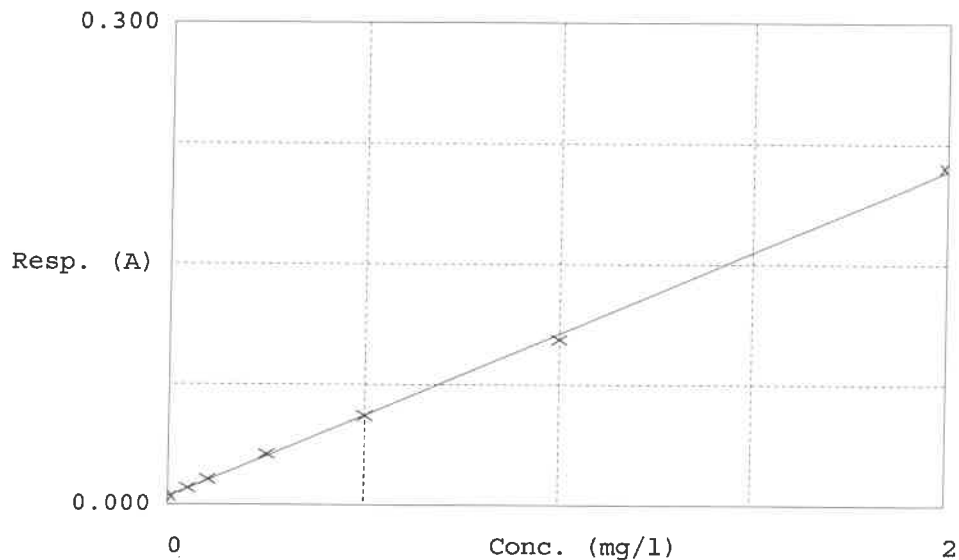

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.005	0.0006	0.0000	-
2	Phenol-2	0.010	0.0528	0.0500	5-6
3	Phenol-2	0.016	0.1067	0.1000	6.7
4	Phenol-2	0.032	0.2620	0.2500	4.8
5	Phenol-2	0.055	0.4967	0.5000	-0.7
6	Phenol-2	0.103	0.9644	1.0000	-3.6
7	Phenol-2	0.210	2.0167	2.0000	0.8

05/30/2024
RM