


LB131005

7471B

INSTRUMENT ID: CV1

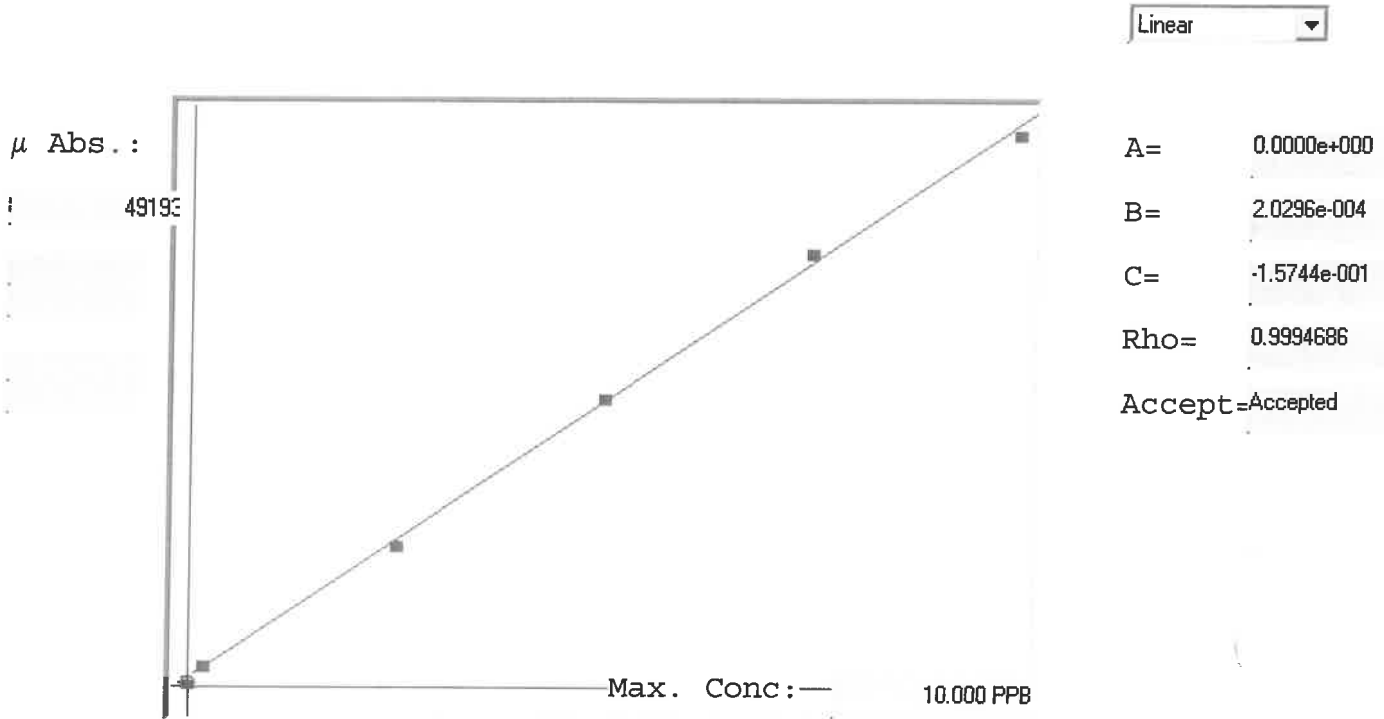

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	(%)
0.0	0.000	-0.060	-0.060	482	0.000	482					1
0.2	0.200	0.245	0.045	1982	0.0 %	1982					23
2.5	2.500	2.414	-0.086	12672	0.0 %	12672					3
5.0	5.000	5.080	0.080	25808	0.0 %	25808					2
7.5	7.500	7.693	0.193	38682	0.0 %	38682					3
10.0	10.000	9.827	-0.173	49193	0.0 %	49193					2

LB131005 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 31 May 2024 10:22:13

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	482	-	0.0000	7471B	PPB	31 May 2024 10:32:55	S	Std
0.2 - 1	50.2	1982	-	0.2000	7471B	PPB	31 May 2024 10:35:12	S	Std
2.5 - 1	52.5	12672	-	2.5000	7471B	PPB	31 May 2024 10:37:29	S	Std
5.0 - 1	55	25808	-	5.0000	7471B	PPB	31 May 2024 10:39:46	S	Std
7.5 - 1	57.5	38682	-	7.5000	7471B	PPB	31 May 2024 10:42:05	S	Std
10.0 - 1	510	49193	-	10.0000	7471B	PPB	31 May 2024 10:47:04	S	Std
ICV69 - 1	ICV69	20193	3.9409	-	7471B	PPB	31 May 2024 10:50:01	U	SMPL
ICB69 - 1	ICB69	692	-0.0170	-	7471B	PPB	31 May 2024 10:52:17	U	SMPL
CCV63 - 1	CCV63	26505	5.2219	-	7471B	PPB	31 May 2024 10:54:35	U	SMPL
CCB63 - 1	CCB63	796	0.0041	-	7471B	PPB	31 May 2024 10:56:50	U	SMPL
CRA - 1	CRA	2010	0.2505	-	7471B	PPB	31 May 2024 10:59:15	U	SMPL
HighStd - 1	HighStd	50881	10.1692	-	7471B	PPB	31 May 2024 11:01:30	U	SMPL
ChkStd - 1	ChkStd	35934	7.1356	-	7471B	PPB	31 May 2024 11:03:46	U	SMPL
PB161230BL - 1	PBS	486	-0.0588	-	7471B	PPB	31 May 2024 11:12:16	U	SMPL
PB161230BS - 1	LCSS	19810	3.8631	-	7471B	PPB	31 May 2024 11:17:05	U	SMPL
P2610-01 - 1	HR-01-05242024	6569	1.1758	-	7471B	PPB	31 May 2024 11:19:22	U	SMPL
P2610-01DUP - 1	HR-01-05242024DUP	6476	1.1569	-	7471B	PPB	31 May 2024 11:21:41	U	SMPL
P2610-01MS - 1	HR-01-05242024MS	23161	4.5432	-	7471B	PPB	31 May 2024 11:24:01	U	SMPL
P2610-01MSD - 1	HR-01-05242024MSD	22013	4.3102	-	7471B	PPB	31 May 2024 11:26:21	U	SMPL
P2610-03 - 1	HR-02-05242024	2041	0.2568	-	7471B	PPB	31 May 2024 11:28:40	U	SMPL
CCV64 - 1	CCV64	25243	4.9658	-	7471B	PPB	31 May 2024 11:30:59	U	SMPL
CCB64 - 1	CCB64	680	-0.0194	-	7471B	PPB	31 May 2024 11:33:16	U	SMPL
P2637-01 - 1	WCS-TPT	2921	0.4354	-	7471B	PPB	31 May 2024 11:35:35	U	SMPL
P2646-01 - 1	WCS-TPS	2620	0.3743	-	7471B	PPB	31 May 2024 11:37:50	U	SMPL
P2654-01 - 1	OR-03-052924	4388	0.7331	-	7471B	PPB	31 May 2024 11:40:07	U	SMPL
P2655-01 - 1	EO-02-052924	7361	1.3365	-	7471B	PPB	31 May 2024 11:42:24	U	SMPL
P2657-01 - 1	1-AB	12420	2.3633	-	7471B	PPB	31 May 2024 11:44:42	U	SMPL
P2657-05 - 1	2-AB	9845	1.8407	-	7471B	PPB	31 May 2024 11:47:01	U	SMPL
P2657-09 - 1	3-AB	5995	1.0593	-	7471B	PPB	31 May 2024 11:49:20	U	SMPL
P2657-13 - 1	4-AB	6537	1.1693	-	7471B	PPB	31 May 2024 11:51:40	U	SMPL
P2657-17 - 1	5-AB	3130	0.4778	-	7471B	PPB	31 May 2024 11:53:59	U	SMPL
P2662-01 - 1	WCS-TPR	851	0.0153	-	7471B	PPB	31 May 2024 11:56:16	U	SMPL
CCV65 - 1	CCV65	25547	5.0275	-	7471B	PPB	31 May 2024 11:58:33	U	SMPL
CCB65 - 1	CCB65	769	-0.0014	-	7471B	PPB	31 May 2024 12:00:49	U	SMPL
P2610-01LX5 - 1		1349	0.1163	-	7471B	PPB	31 May 2024 12:03:07	U	SMPL
P2610-01A - 1		28512	5.6293	-	7471B	PPB	31 May 2024 12:05:22	U	SMPL
CCV66 - 1	CCV66	25585	5.0352	-	7471B	PPB	31 May 2024 12:10:17	U	SMPL
CCB66 - 1	CCB66	762	-0.0028	-	7471B	PPB	31 May 2024 12:12:32	U	SMPL