


LB131016

SFAM01.1

INSTRUMENT ID: CV1

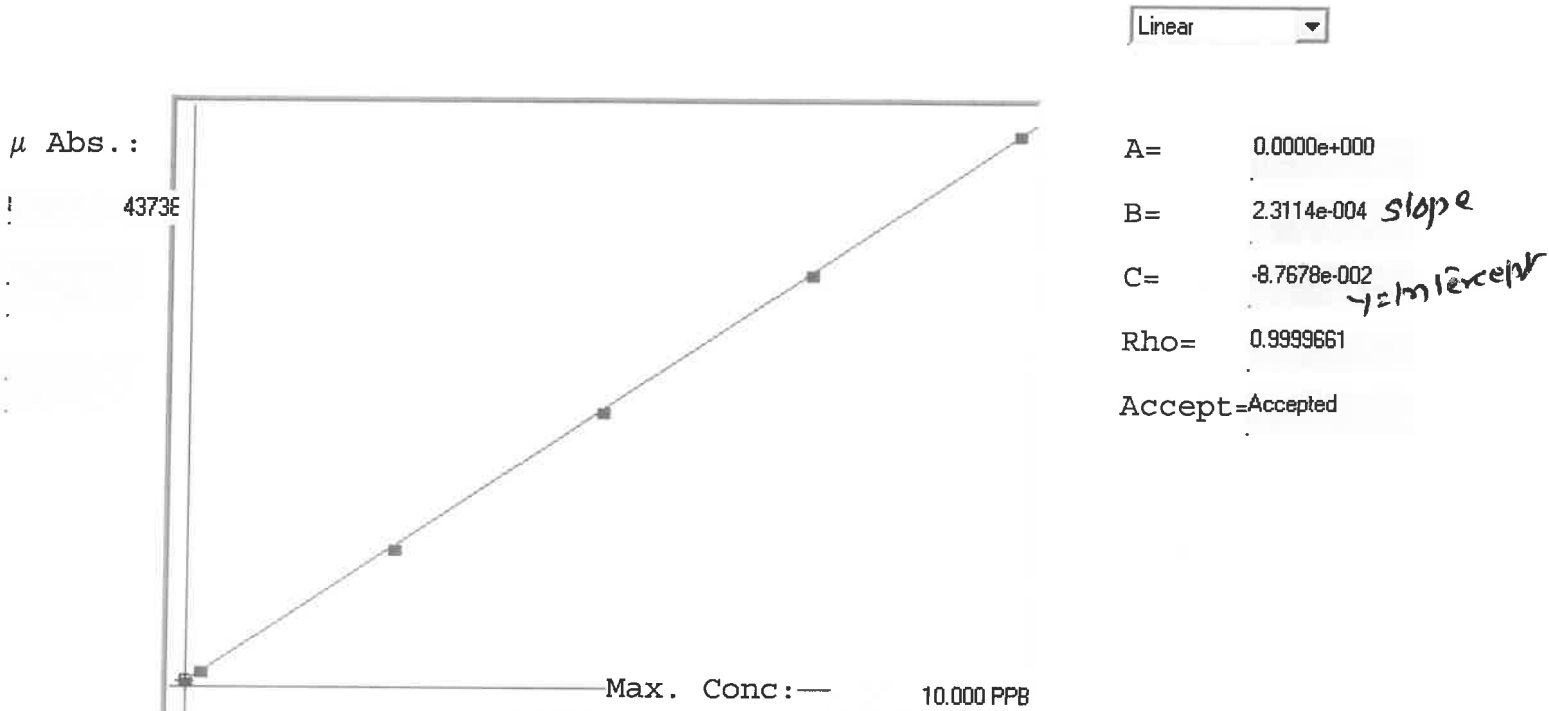

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.030	0.030	510	0.000	510					
0.05	0.050					442					
0.20	0.200	0.223	0.023	1343	0.0 %	1343	0				
2.50	2.500	2.443	-0.057	10947	0.0 %	10947					
5.00	5.000	4.982	-0.018	21933	0.0 %	21933					
7.50	7.500	7.501	0.001	32832	0.0 %	32832					
10.0	10.000	10.022	0.022	43738	0.0 %	43738					

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc.	Method	Units	Date	Type
	0 S0	510	-		0 SFAM01.1	PPB	5/31/2024 15:30	Std
	0.2 S01	1343	-		0.2 SFAM01.1	PPB	5/31/2024 15:33	Std
	2.5 S02	10947	-		2.5 SFAM01.1	PPB	5/31/2024 15:35	Std
	5 S03	21933	-		5 SFAM01.1	PPB	5/31/2024 15:37	Std
	7.5 S04	32832	-		7.5 SFAM01.1	PPB	5/31/2024 15:40	Std
	10 S05	43738	-		10 SFAM01.1	PPB	5/31/2024 15:42	Std
ICV071	ICV071	18594	4.2101	-	SFAM01.1	PPB	5/31/2024 15:51	SMPL
ICB071	ICB071	701	0.0743	-	SFAM01.1	PPB	5/31/2024 15:53	SMPL
CCV069	CCV069	22314	5.0699	-	SFAM01.1	PPB	5/31/2024 15:55	SMPL
CCB069	CCB069	396	0.0039	-	SFAM01.1	PPB	5/31/2024 15:58	SMPL
PB161244BL	PBS244	461	0.0189	-	SFAM01.1	PPB	5/31/2024 16:03	SMPL
P2592-02	MBH5S3	4759	1.0123	-	SFAM01.1	PPB	5/31/2024 16:05	SMPL
P2592-03	MBH5S4	5817	1.2568	-	SFAM01.1	PPB	5/31/2024 16:07	SMPL
P2592-04	MBH5S5	6013	1.3021	-	SFAM01.1	PPB	5/31/2024 16:09	SMPL
P2592-05	MBH5S5D	5592	1.2048	-	SFAM01.1	PPB	5/31/2024 16:12	SMPL
P2592-06	MBH5S5S	18000	4.0728	-	SFAM01.1	PPB	5/31/2024 16:14	SMPL
P2592-07	MBH5S6	9169	2.0316	-	SFAM01.1	PPB	5/31/2024 16:16	SMPL
P2592-08	MBH5S7	10711	2.388	-	SFAM01.1	PPB	5/31/2024 16:18	SMPL
P2592-09	MBH5T8	16569	3.742	-	SFAM01.1	PPB	5/31/2024 16:21	SMPL
P2592-10	MBH5T9	23555	5.3567	-	SFAM01.1	PPB	5/31/2024 16:23	SMPL
P2592-11	MBH5W1	15671	3.5344	-	SFAM01.1	PPB	5/31/2024 16:25	SMPL
P2592-12	MBH6D7	7908	1.7401	-	SFAM01.1	PPB	5/31/2024 16:28	SMPL
P2592-13	MBH6D8	82883	19.0695	-	SFAM01.1	PPB	5/31/2024 16:30	SMPL
P2592-14	MBH6D9	145065	33.442	-	SFAM01.1	PPB	5/31/2024 16:32	SMPL
P2592-15	MBH6E0	136982	31.5737	-	SFAM01.1	PPB	5/31/2024 16:34	SMPL
P2592-16	MBH6E1	43285	9.917	-	SFAM01.1	PPB	5/31/2024 16:37	SMPL
P2592-17	MBH6E2	26685	6.0802	-	SFAM01.1	PPB	5/31/2024 16:39	SMPL
P2592-18	MBH6E3	7848	1.7263	-	SFAM01.1	PPB	5/31/2024 16:42	SMPL
P2592-19	MBH6E4	18546	4.199	-	SFAM01.1	PPB	5/31/2024 16:44	SMPL
P2592-20	MBH6E5	7320	1.6042	-	SFAM01.1	PPB	5/31/2024 16:46	SMPL
CCV070	CCV070	21907	4.9758	-	SFAM01.1	PPB	5/31/2024 16:48	SMPL
CCB070	CCB070	242	-0.0317	-	SFAM01.1	PPB	5/31/2024 16:51	SMPL
P2592-21	MBH6E6	6032	1.3065	-	SFAM01.1	PPB	5/31/2024 16:53	SMPL
PB161245BL	PBS245	213	-0.0384	-	SFAM01.1	PPB	5/31/2024 16:55	SMPL
P2593-01	MBH5W2	9033	2.0002	-	SFAM01.1	PPB	5/31/2024 16:58	SMPL
P2593-02	MBH5W3	6584	1.4341	-	SFAM01.1	PPB	5/31/2024 17:00	SMPL
P2593-03	MBH5W4	10831	2.4158	-	SFAM01.1	PPB	5/31/2024 17:02	SMPL
P2593-04	MBH5W5	13356	2.9994	-	SFAM01.1	PPB	5/31/2024 17:04	SMPL
P2593-05	MBH5W5D	15065	3.3944	-	SFAM01.1	PPB	5/31/2024 17:07	SMPL
P2593-06	MBH5W5S	24004	5.4605	-	SFAM01.1	PPB	5/31/2024 17:12	SMPL
P2593-07	MBH5W6	9945	2.211	-	SFAM01.1	PPB	5/31/2024 17:14	SMPL
P2593-08	MBH5W7	3726	0.7735	-	SFAM01.1	PPB	5/31/2024 17:16	SMPL
P2593-09	MBH6C3	22960	5.2192	-	SFAM01.1	PPB	5/31/2024 17:19	SMPL
P2593-10	MBH6C4	15903	3.5881	-	SFAM01.1	PPB	5/31/2024 17:21	SMPL
P2593-11	MBH6C5	9944	2.2107	-	SFAM01.1	PPB	5/31/2024 17:23	SMPL
P2593-12	MBH6C6	9179	2.0339	-	SFAM01.1	PPB	5/31/2024 17:25	SMPL

LB131016

INSTRUMENT ID : CV1

P2593-13	MBH6C7	11074	2.4719 -	SFAM01.1	PPB	5/31/2024 17:28 SMPL
P2593-14	MBH6C8	24959	5.6812 -	SFAM01.1	PPB	5/31/2024 17:30 SMPL
P2593-15	MBH6C9	13126	2.9462 -	SFAM01.1	PPB	5/31/2024 17:32 SMPL
P2593-16	MBH6D0	15840	3.5735 -	SFAM01.1	PPB	5/31/2024 17:35 SMPL
P2593-17	MBH6D1	11042	2.4645 -	SFAM01.1	PPB	5/31/2024 17:37 SMPL
P2593-18	MBH6D2	33552	7.6674 -	SFAM01.1	PPB	5/31/2024 17:39 SMPL
CCV071	CCV071	22048	5.0084 -	SFAM01.1	PPB	5/31/2024 17:41 SMPL
CCB071	CCB071	91	-0.0666 -	SFAM01.1	PPB	5/31/2024 17:44 SMPL
P2593-19	MBH6D3	26940	6.1391 -	SFAM01.1	PPB	5/31/2024 17:46 SMPL
P2593-20	MBH6D4	21825	4.9569 -	SFAM01.1	PPB	5/31/2024 17:48 SMPL
P2593-21	MBH6D5	12144	2.7192 -	SFAM01.1	PPB	5/31/2024 17:51 SMPL
P2593-22	MBH6D6	11616	2.5972 -	SFAM01.1	PPB	5/31/2024 17:53 SMPL
P2592-13DLX5	MBH6D8	16951	3.8303 -	SFAM01.1	PPB	5/31/2024 17:55 SMPL
P2592-14DLX10	MBH6D9	12774	2.8648 -	SFAM01.1	PPB	5/31/2024 17:57 SMPL
P2592-15DLX10	MBH6E0	15599	3.5178 -	SFAM01.1	PPB	5/31/2024 18:00 SMPL
CCV072	CCV072	22241	5.053 -	SFAM01.1	PPB	5/31/2024 18:02 SMPL
CCB072	CCB072	64	-0.0729 -	SFAM01.1	PPB	5/31/2024 18:04 SMPL