

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A


ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio n HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-051324	5/13/2024 15:40		IZ/MA
STD2	0.4450	0.6690	0.6700	2.1990	0.5620	1.1310	3.4510	IC1-051324	5/13/2024 16:02		IZ/MA
STD3	0.8040	1.2260	1.2290	4.0910	1.0210	1.9980	6.1260	IC1-051324	5/13/2024 16:23		IZ/MA
STD4	1.0000	1.4810	1.4990	4.9540	1.2400	2.5220	7.4370	IC1-051324	5/13/2024 16:45		IZ/MA
STD5	1.9530	2.9200	2.8930	9.7290	2.4170	4.8420	14.4330	IC1-051324	5/13/2024 17:06		IZ/MA
STD6	3.9170	5.8890	5.8830	19.6980	4.9170	9.7880	29.2960	IC1-051324	5/13/2024 17:27		IZ/MA
STD7	5.0810	7.6150	7.6260	25.3280	6.3430	12.7180	37.7560	IC1-051324	5/13/2024 17:49		IZ/MA

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	11.2500	11.5000	11.6667	9.9500	12.4000	13.1000	15.0333
STD3	0.5000	2.1667	2.4167	2.2750	2.1000	-0.1000	2.1000
STD4	0.0000	-1.2667	-0.0667	-0.9200	-0.8000	0.8800	-0.8400
STD5	-2.3500	-2.6667	-3.5667	-2.7100	-3.3200	-3.1600	-3.7800
STD6	-2.0750	-1.8500	-1.9500	-1.5100	-1.6600	-2.1200	-2.3467
STD7	1.6200	1.5333	1.6800	1.3120	1.4880	1.7440	2.0432

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

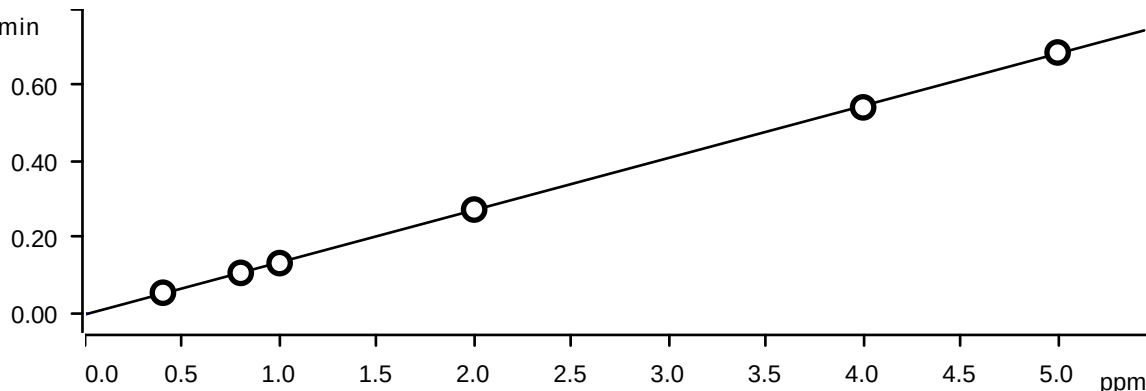

Function: $A = -3.05003E-3 + 0.0137350 \times Q$


Relative standard deviation 1.034950 %

Correlation coefficient 0.999943

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.054	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.106	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.132	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.273	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.542	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.687	Std 7	2024-04-13 01:04:41 UTC-4	used

Chloride (Anions)


($\mu\text{S}/\text{cm}$) x min

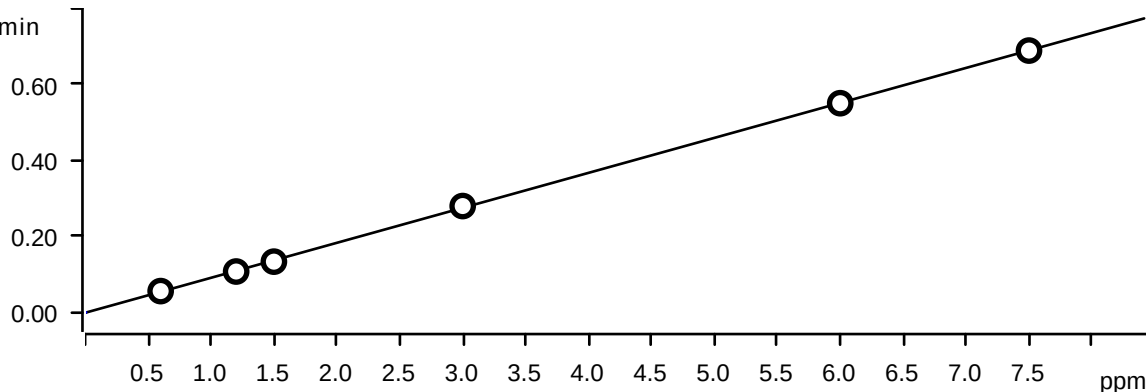

Function: $A = -1.03082E-3 + 9.21146E-3 \times Q$

Relative standard deviation 1.071537 %
Correlation coefficient 0.999938


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.056	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.108	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.134	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.280	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.551	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.689	Std 7	2024-04-13 01:04:41 UTC-4	used

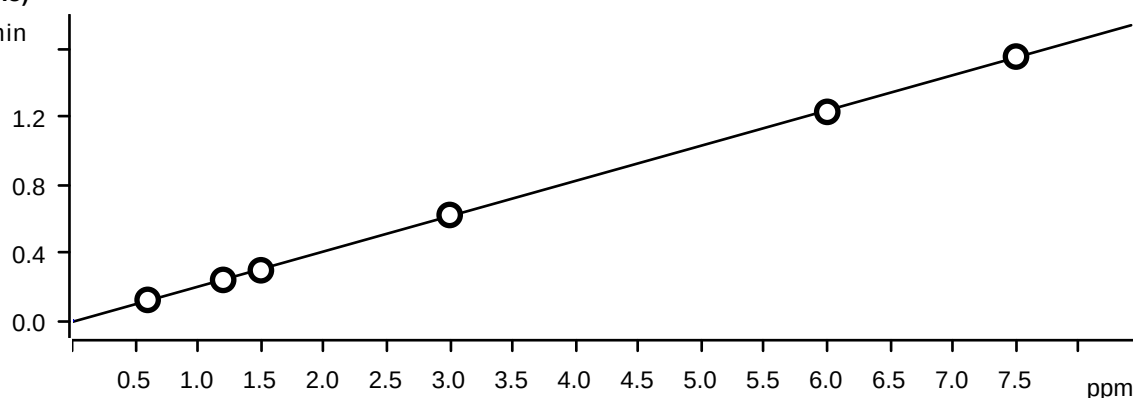Nitrite (Anions) $(\mu\text{S/cm}) \times \text{min}$ 

Function: $A = -8.19751E-3 + 0.0207534 \times Q$
Relative standard deviation 1.139145 %
Correlation coefficient 0.999931

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.122	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.239	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.296	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.621	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.228	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.554	Std 7	2024-04-13 01:04:41 UTC-4	used

Bromide (Anions)

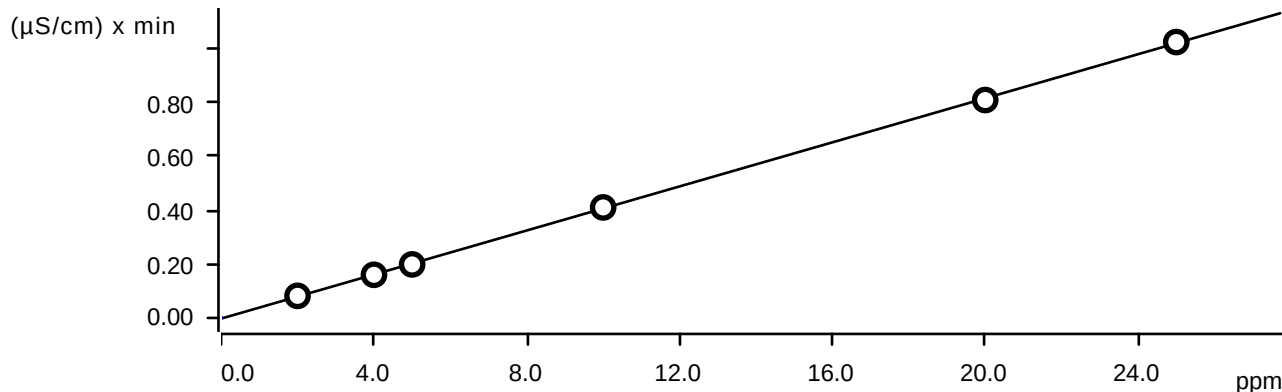


Function: $A = -2.93159E-3 + 4.09511E-3 \times Q$

Relative standard deviation: 1.087762 %

Correlation coefficient: 0.999936

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.082	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.160	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.199	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.410	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.810	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.025	Std 7	2024-04-13 01:04:41 UTC-4	used

Nitrate (Anions)

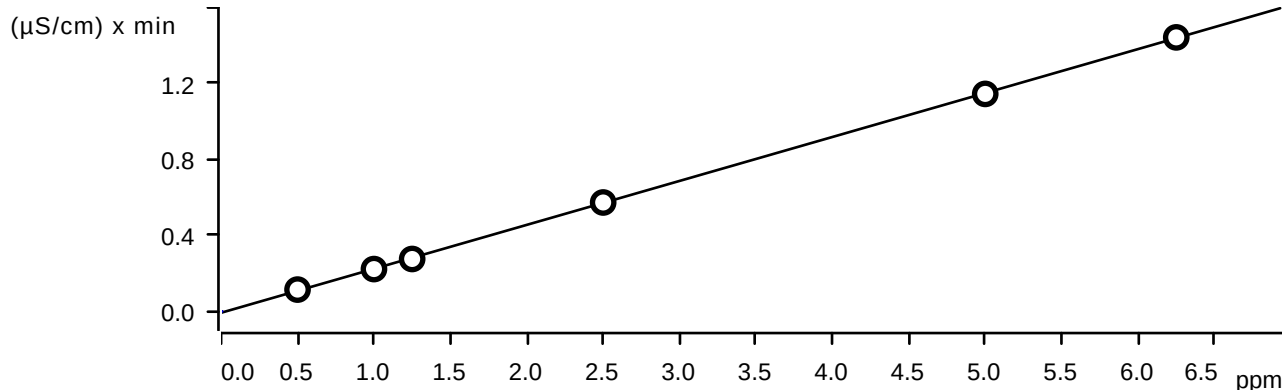


Function: $A = -7.15004E-3 + 0.0231424 \times Q$

Relative standard deviation: 0.870938 %

Correlation coefficient 0.999960


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.115	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.223	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.276	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.573	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.145	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.443	Std 7	2024-04-13 01:04:41 UTC-4	used

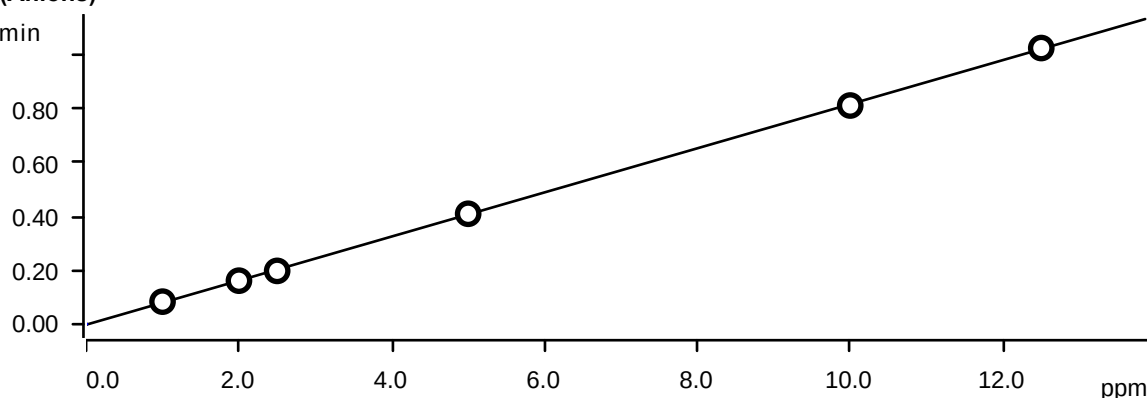Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -2.37452E-3 + 8.19864E-3 \times Q$

Relative standard deviation 1.011855 %

Correlation coefficient 0.999945

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.083	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.161	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.198	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.410	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.813	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.026	Std 7	2024-04-13 01:04:41 UTC-4	used

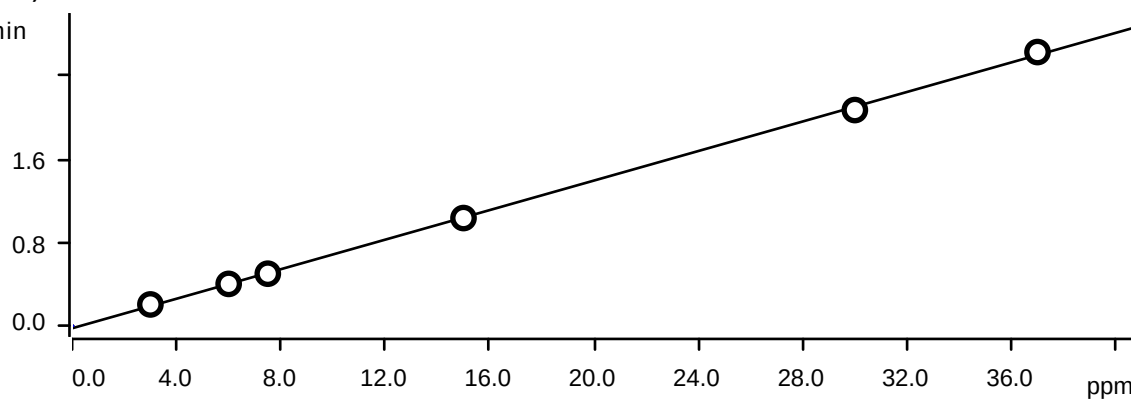Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0233221 + 7.09240E-3 \times Q$

Relative standard deviation 2.047074 %

Correlation coefficient 0.999778

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	Std 1	2024-04-12 22:45:19 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.206	Std 2	2024-04-12 23:06:41 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.403	Std 3	2024-04-12 23:38:39 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.501	Std 4	2024-04-13 00:00:33 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.035	Std 5	2024-04-13 00:21:58 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.072	Std 6	2024-04-13 00:43:14 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.629	Std 7	2024-04-13 01:04:41 UTC-4	used


Sample data

Ident Std 1
Sample type Standard 1
Determination start 2024-04-12 22:45:19 UTC-4
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

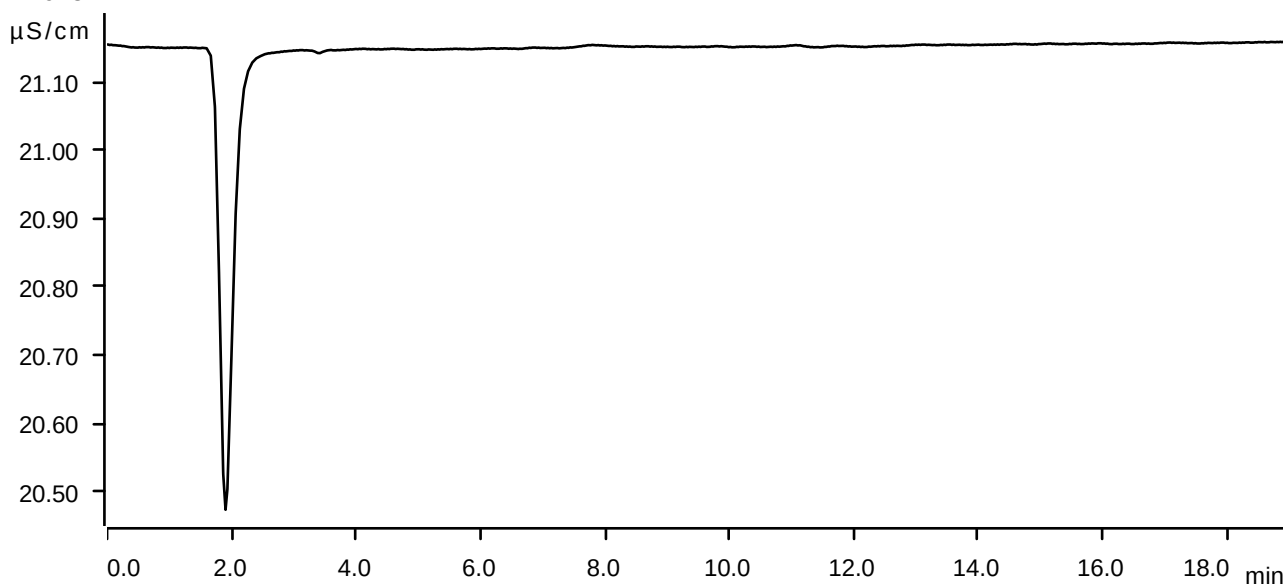


Sample data

Ident Std 2
Sample type Standard 2
Determination start 2024-04-12 23:06:41 UTC-4
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

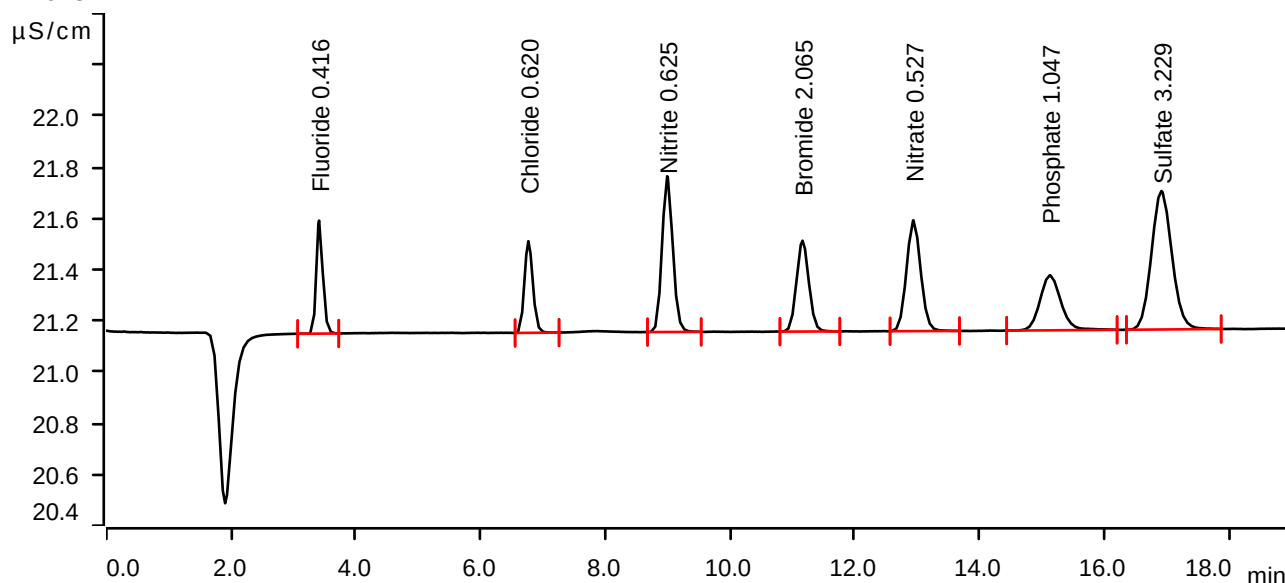

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.412	0.0541	0.441	0.416	Fluoride
2	6.767	0.0561	0.358	0.620	Chloride
3	8.993	0.1216	0.608	0.625	Nitrite
4	11.162	0.0816	0.355	2.065	Bromide
5	12.940	0.1148	0.433	0.527	Nitrate
6	15.127	0.0834	0.215	1.047	Phosphate
7	16.915	0.2057	0.541	3.229	Sulfate


Sample data

Ident Std 3
Sample type Standard 3
Determination start 2024-04-12 22:38:39 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.5 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

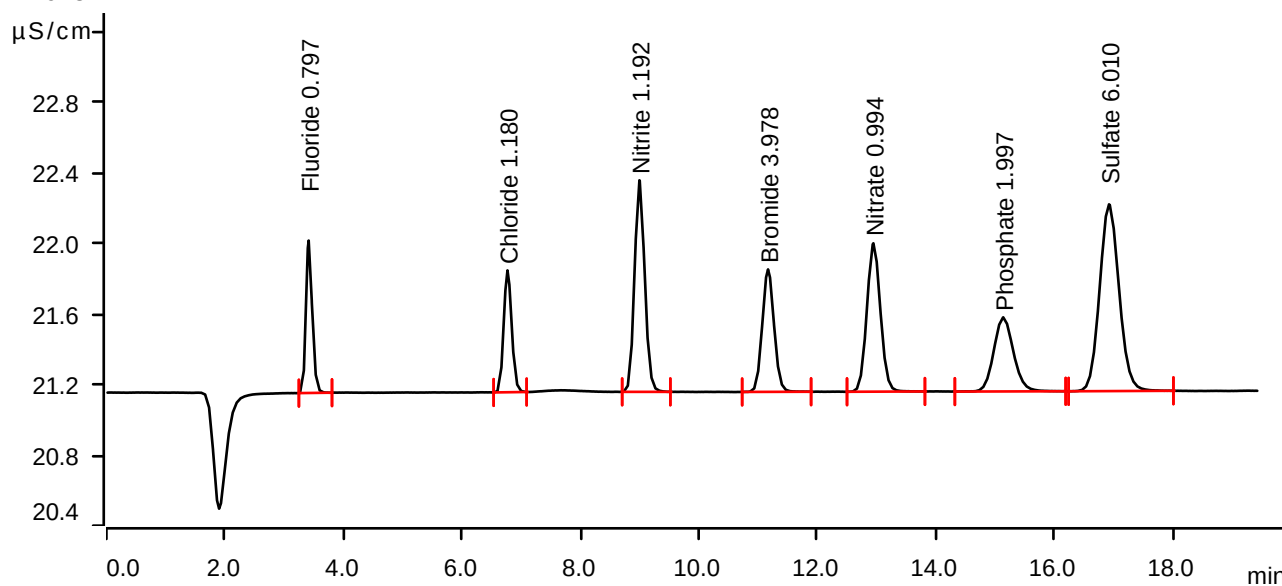

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.415	0.1064	0.863	0.797	Fluoride
2	6.770	0.1076	0.690	1.180	Chloride
3	8.997	0.2391	1.198	1.192	Nitrite
4	11.167	0.1600	0.694	3.978	Bromide
5	12.945	0.2229	0.840	0.994	Nitrate
6	15.137	0.1614	0.420	1.997	Phosphate
7	16.922	0.4029	1.057	6.010	Sulfate


Sample data

Ident Std 4
Sample type Standard 4
Determination start 2024-04-12 23:00:33 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

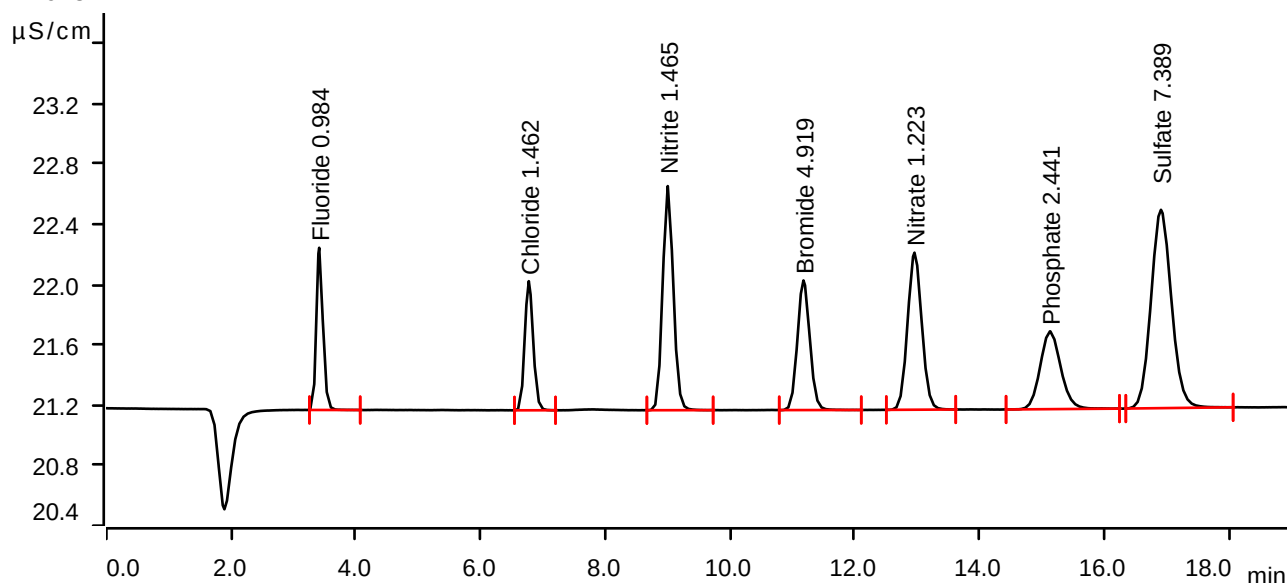

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.413	0.1321	1.077	0.984	Fluoride
2	6.773	0.1336	0.857	1.462	Chloride
3	9.002	0.2959	1.487	1.465	Nitrite
4	11.177	0.1985	0.861	4.919	Bromide
5	12.957	0.2759	1.043	1.223	Nitrate
6	15.128	0.1978	0.517	2.441	Phosphate
7	16.908	0.5007	1.317	7.389	Sulfate


Sample data

Ident Std 5
Sample type Standard 5
Determination start 2024-04-12 23:21:58 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

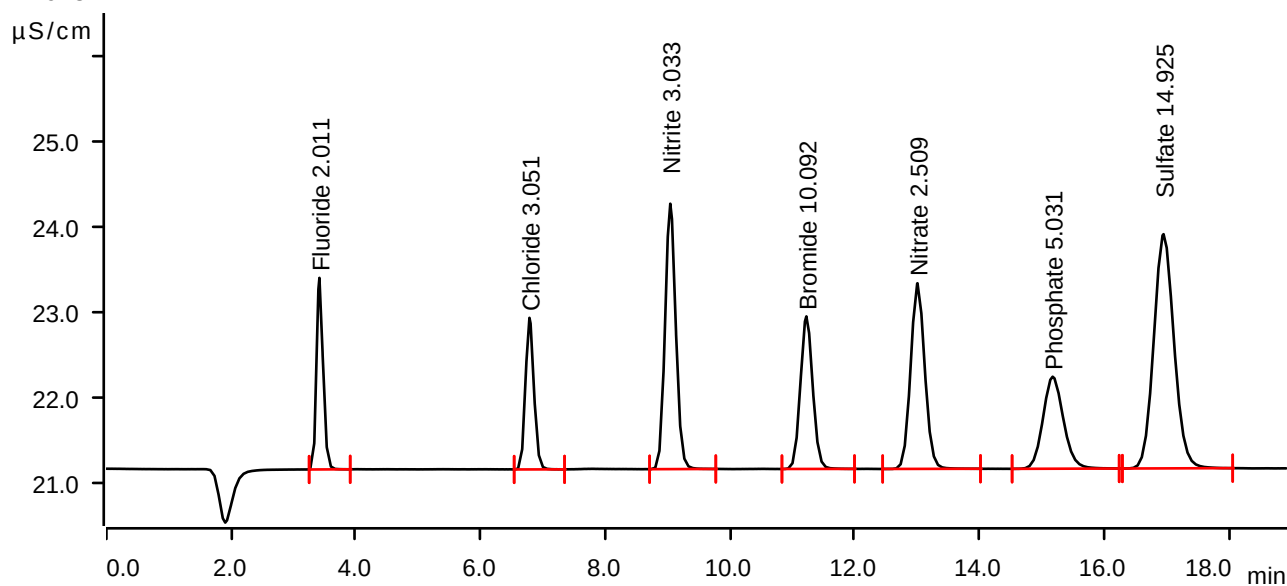

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.417	0.2731	2.244	2.011	Fluoride
2	6.783	0.2800	1.776	3.051	Chloride
3	9.042	0.6213	3.109	3.033	Nitrite
4	11.223	0.4104	1.788	10.092	Bromide
5	13.005	0.5735	2.175	2.509	Nitrate
6	15.172	0.4101	1.078	5.031	Phosphate
7	16.950	1.0352	2.744	14.925	Sulfate


Sample data

Ident Std 6
Sample type Standard 6
Determination start 2024-04-12 23:43:14 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

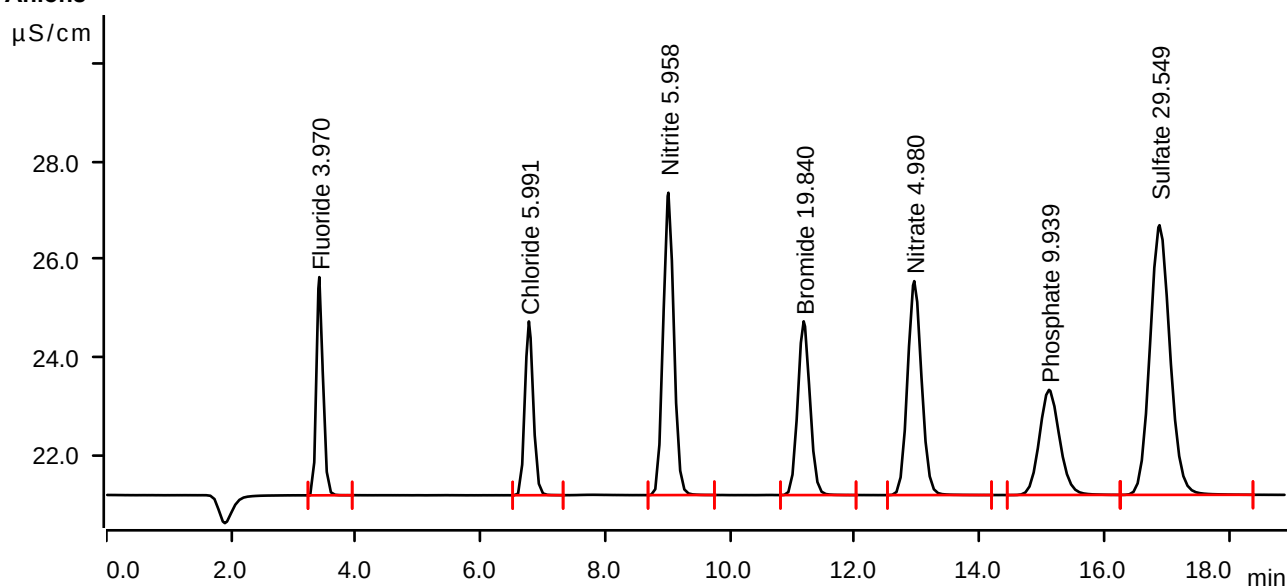

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.415	0.5422	4.473	3.970	Fluoride
2	6.775	0.5509	3.563	5.991	Chloride
3	9.012	1.2283	6.198	5.958	Nitrite
4	11.180	0.8095	3.562	19.840	Bromide
5	12.953	1.1453	4.386	4.980	Nitrate
6	15.113	0.8125	2.155	9.939	Phosphate
7	16.885	2.0724	5.528	29.549	Sulfate


Sample data

Ident Std 7
Sample type Standard 7
Determination start 2024-04-13 00:04:41 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

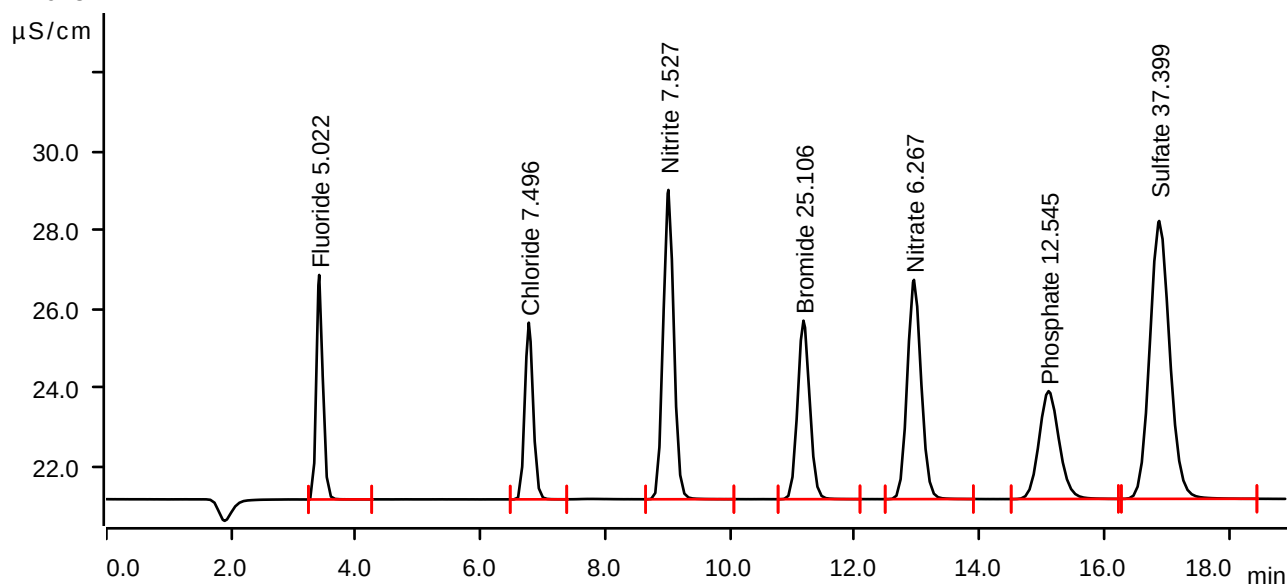

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.413	0.6867	5.697	5.022	Fluoride
2	6.773	0.6894	4.484	7.496	Chloride
3	9.012	1.5538	7.851	7.527	Nitrite
4	11.177	1.0252	4.531	25.106	Bromide
5	12.948	1.4431	5.565	6.267	Nitrate
6	15.107	1.0261	2.739	12.545	Phosphate
7	16.880	2.6292	7.053	37.399	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2024-04-13 02:35:03 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

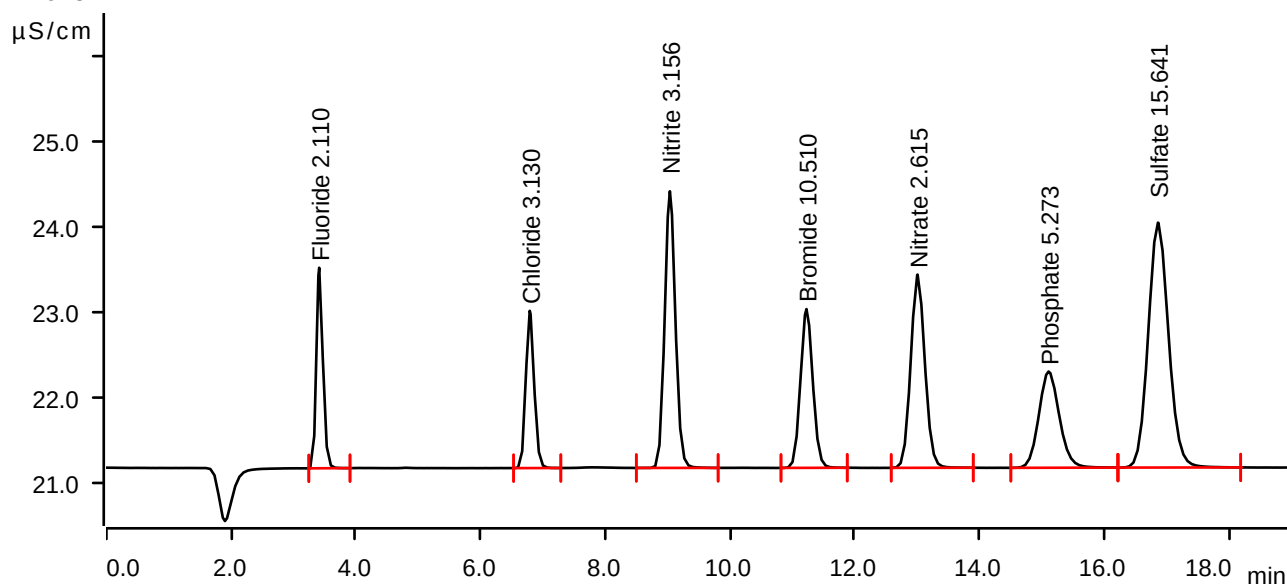

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.413	0.2867	2.349	2.110	Fluoride
2	6.788	0.2873	1.842	3.130	Chloride
3	9.035	0.6468	3.241	3.156	Nitrite
4	11.225	0.4275	1.860	10.510	Bromide
5	13.007	0.5980	2.263	2.615	Nitrate
6	15.107	0.4300	1.127	5.273	Phosphate
7	16.860	1.0860	2.869	15.641	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2024-04-13 02:56:34 UTC-5
Method anions
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

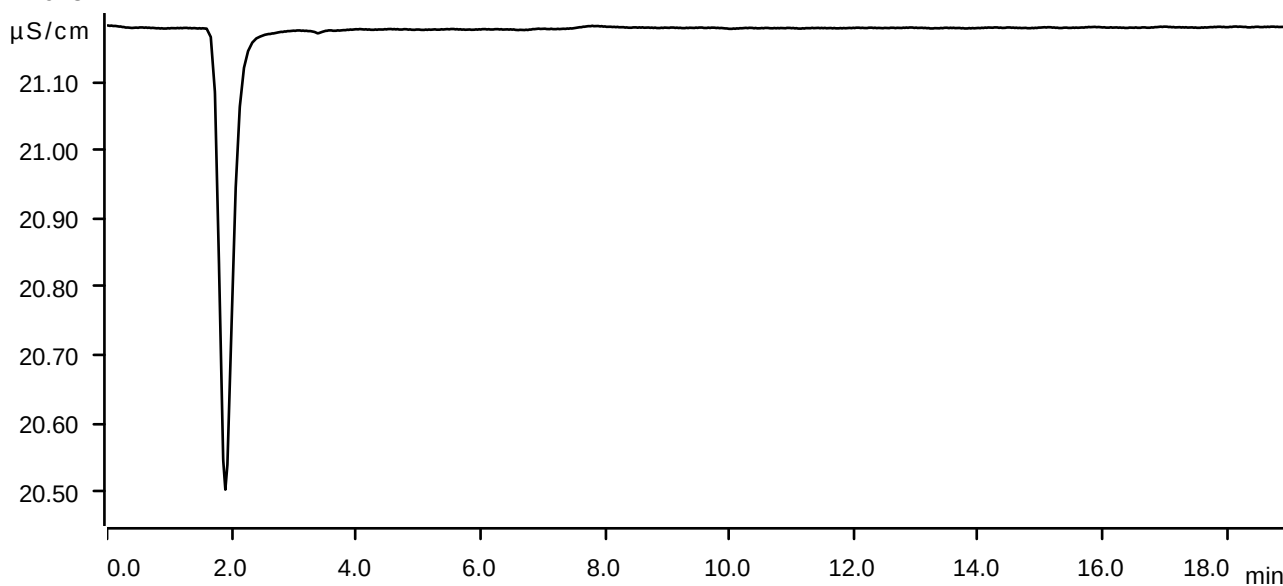


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-06-04 14:38:00 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

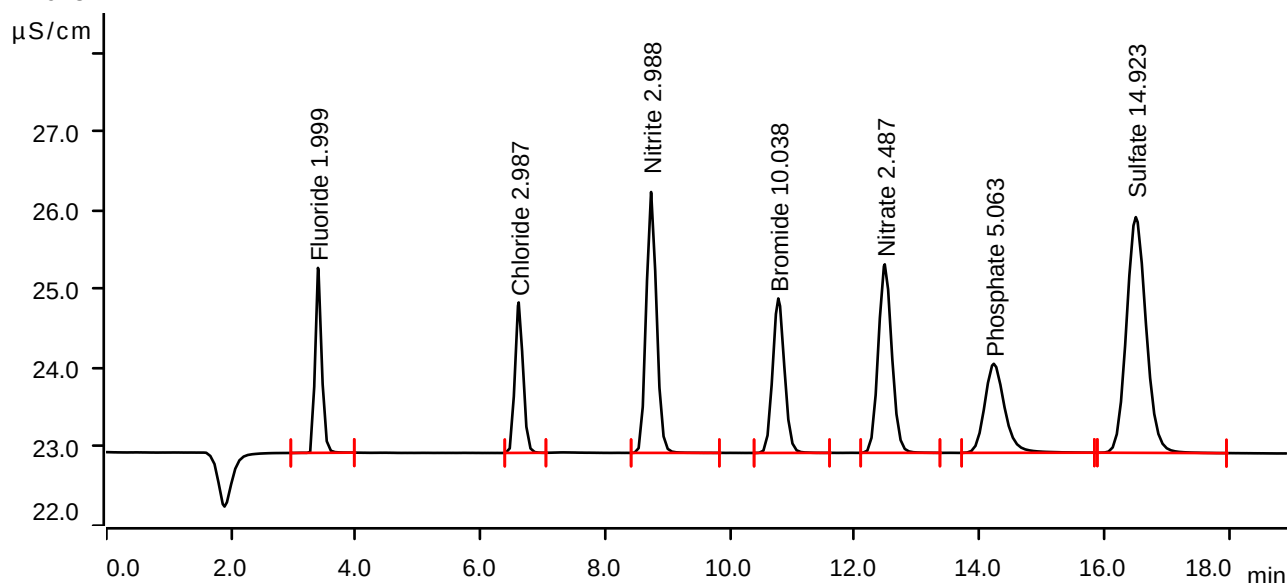

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.2853	2.347	1.999	Fluoride
2	6.612	0.2889	1.909	2.987	Chloride
3	8.735	0.6367	3.310	2.988	Nitrite
4	10.773	0.4316	1.960	10.038	Bromide
5	12.480	0.6027	2.392	2.487	Nitrate
6	14.228	0.4213	1.130	5.063	Phosphate
7	16.505	1.0932	2.991	14.923	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-06-04 14:59:29 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.20 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

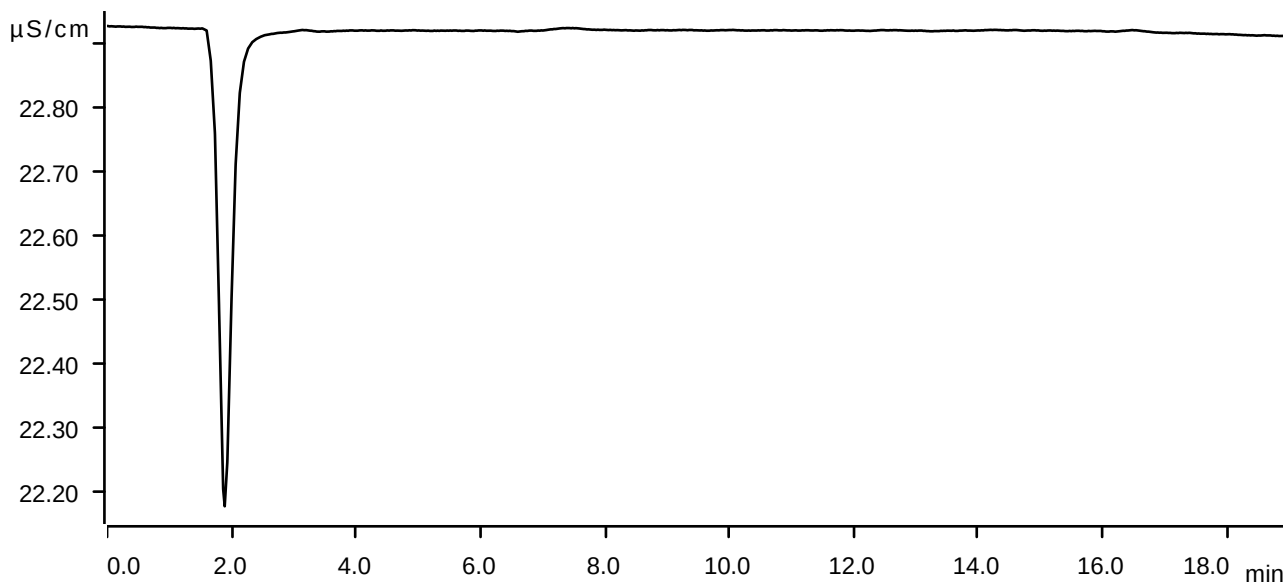


Sample data

Ident LB131061BLW
Sample type Sample
Determination start 2024-06-04 16:28:55 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

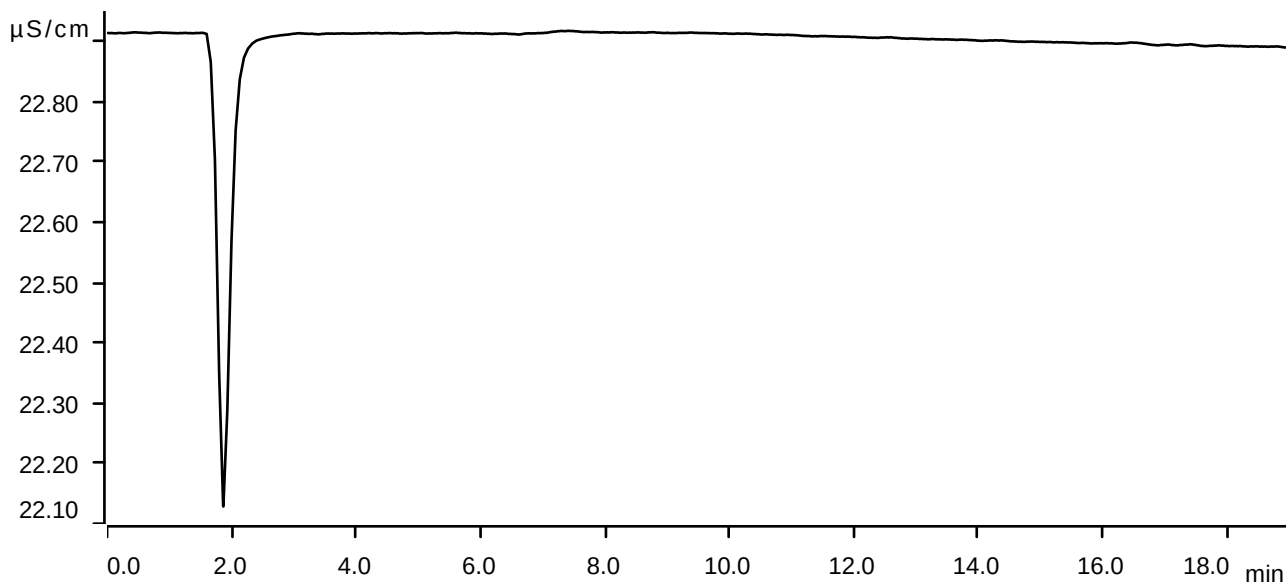Anions


Sample data

Ident LB131061BSW
Sample type Check standard 1
Determination start 2024-06-04 16:50:15 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

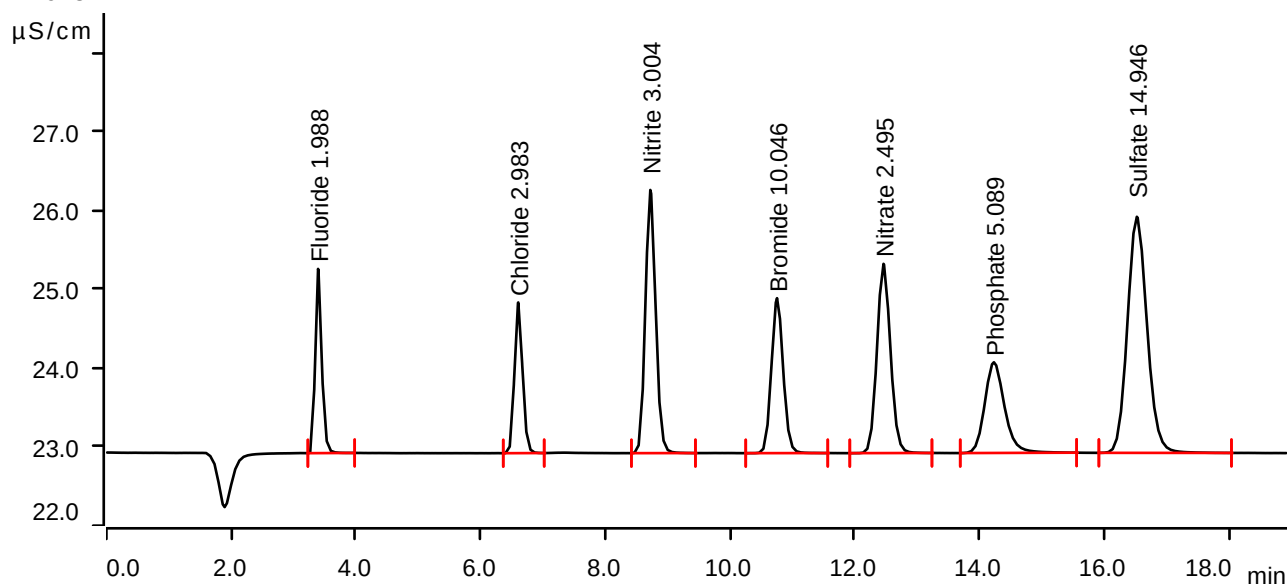

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.395	0.2838	2.338	1.988	Fluoride
2	6.605	0.2885	1.912	2.983	Chloride
3	8.722	0.6402	3.340	3.004	Nitrite
4	10.753	0.4320	1.966	10.046	Bromide
5	12.460	0.6045	2.402	2.495	Nitrate
6	14.230	0.4236	1.151	5.089	Phosphate
7	16.522	1.0949	2.996	14.946	Sulfate


Sample data

Ident P2717-01
Sample type Sample
Determination start 2024-06-04 17:35:08 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

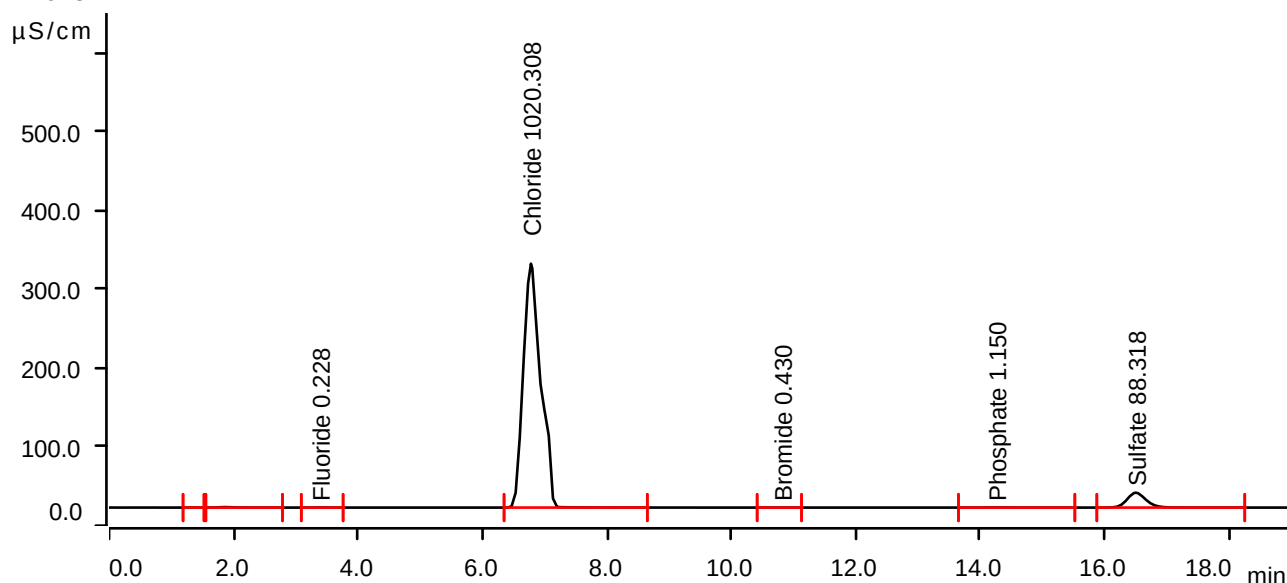

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.355	0.0022	0.014	invalid	
2	1.867	0.1658	0.589	invalid	
3	3.387	0.0275	0.207	0.228	Fluoride
4	6.780	100.3534	309.519	1020.308	Chloride
5	10.812	0.0089	0.040	0.430	Bromide
6	14.257	0.0870	0.222	1.150	Phosphate
7	16.498	6.6656	18.897	88.318	Sulfate


Sample data

Ident P2717-01MS
Sample type Sample
Determination start 2024-06-04 17:58:31 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.29 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

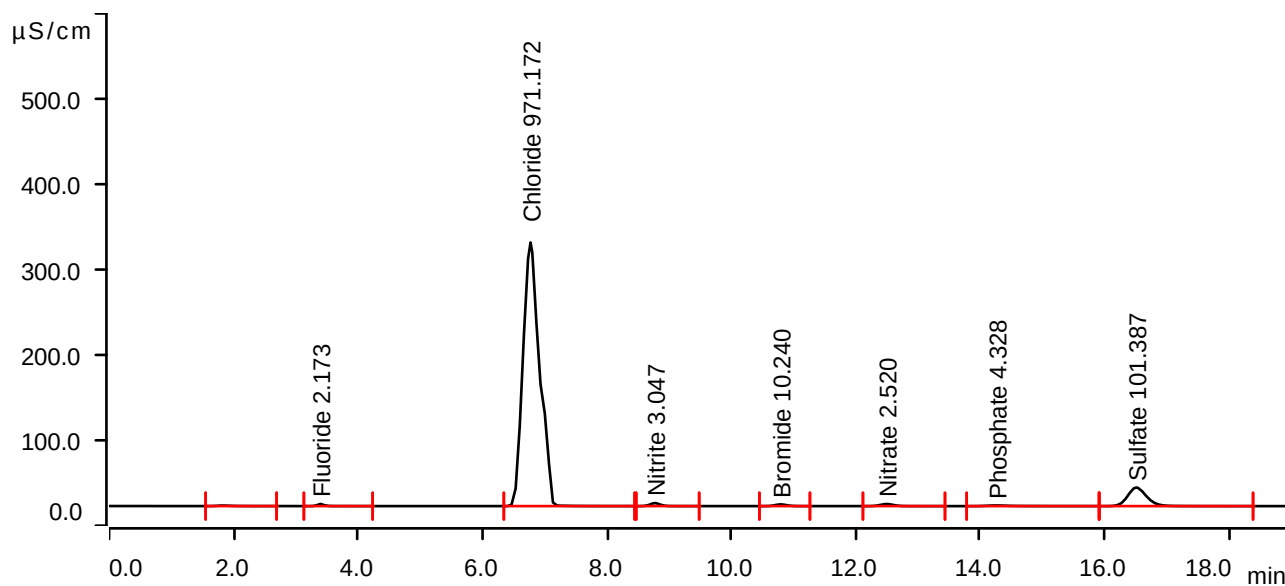

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.835	0.1585	0.619	invalid	
2	3.395	0.3107	2.442	2.173	Fluoride
3	6.773	95.5204	308.744	971.172	Chloride
4	8.770	0.6498	3.499	3.047	Nitrite
5	10.792	0.4405	2.031	10.240	Bromide
6	12.495	0.6108	2.443	2.520	Nitrate
7	14.258	0.3586	0.776	4.328	Phosphate
8	16.507	7.6579	21.777	101.387	Sulfate


Sample data

Ident P2717-01MSD
Sample type Sample
Determination start 2024-06-04 18:20:05 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.98 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

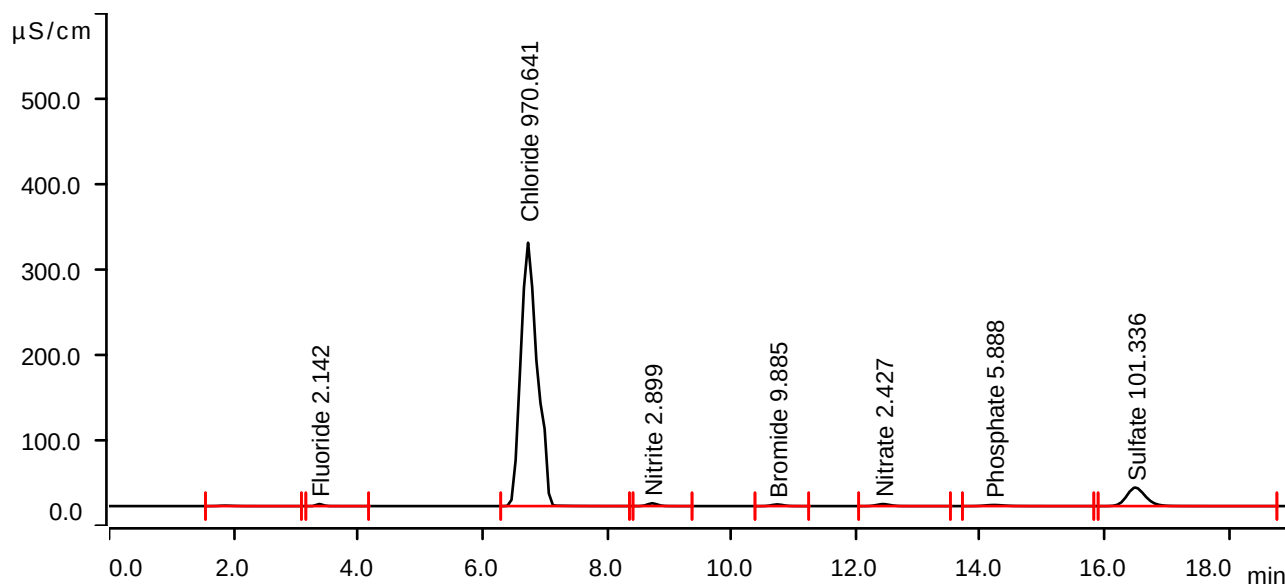

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.863	0.1661	0.574	invalid	
2	3.378	0.3062	2.408	2.142	Fluoride
3	6.735	95.4681	308.488	970.641	Chloride
4	8.728	0.6171	3.298	2.899	Nitrite
5	10.738	0.4249	1.961	9.885	Bromide
6	12.438	0.5876	2.354	2.427	Nitrate
7	14.220	0.4918	1.294	5.888	Phosphate
8	16.492	7.6540	21.722	101.336	Sulfate


Sample data

Ident P2717-02
Sample type Sample
Determination start 2024-06-04 18:41:39 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

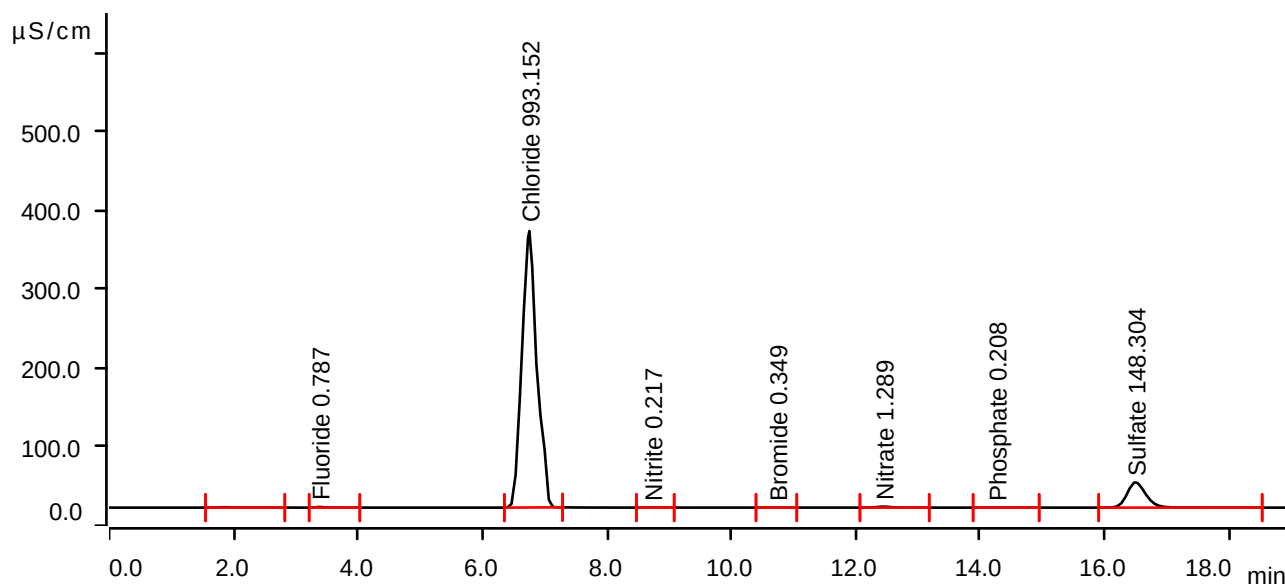

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	1.872	0.1390	0.469	invalid	
2	3.383	0.1090	0.856	0.787	Fluoride
3	6.755	97.6823	350.870	993.152	Chloride
4	8.730	0.0257	0.138	0.217	Nitrite
5	10.738	0.0053	0.025	0.349	Bromide
6	12.447	0.3057	1.220	1.289	Nitrate
7	14.260	0.0066	0.017	0.208	Phosphate
8	16.495	11.2201	32.095	148.304	Sulfate


Sample data

Ident P2717-03
Sample type Sample
Determination start 2024-06-04 19:03:13 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.98 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

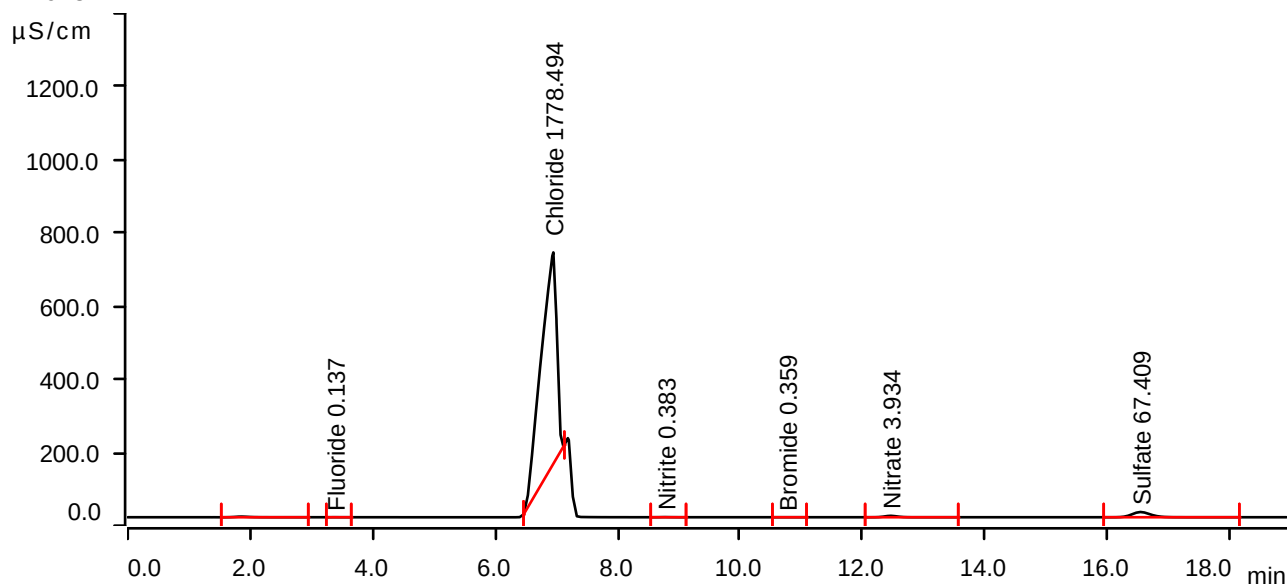

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.852	0.4948	1.791	invalid	
2	3.383	0.0144	0.109	0.137	Fluoride
3	6.950	174.9291	577.628	1778.494	Chloride
4	8.778	0.0624	0.339	0.383	Nitrite
5	10.762	0.0058	0.027	0.359	Bromide
6	12.457	0.9612	3.884	3.934	Nitrate
7	16.537	5.0781	14.339	67.409	Sulfate


Sample data

Ident P2718-01
Sample type Sample
Determination start 2024-06-04 19:24:46 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.87 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

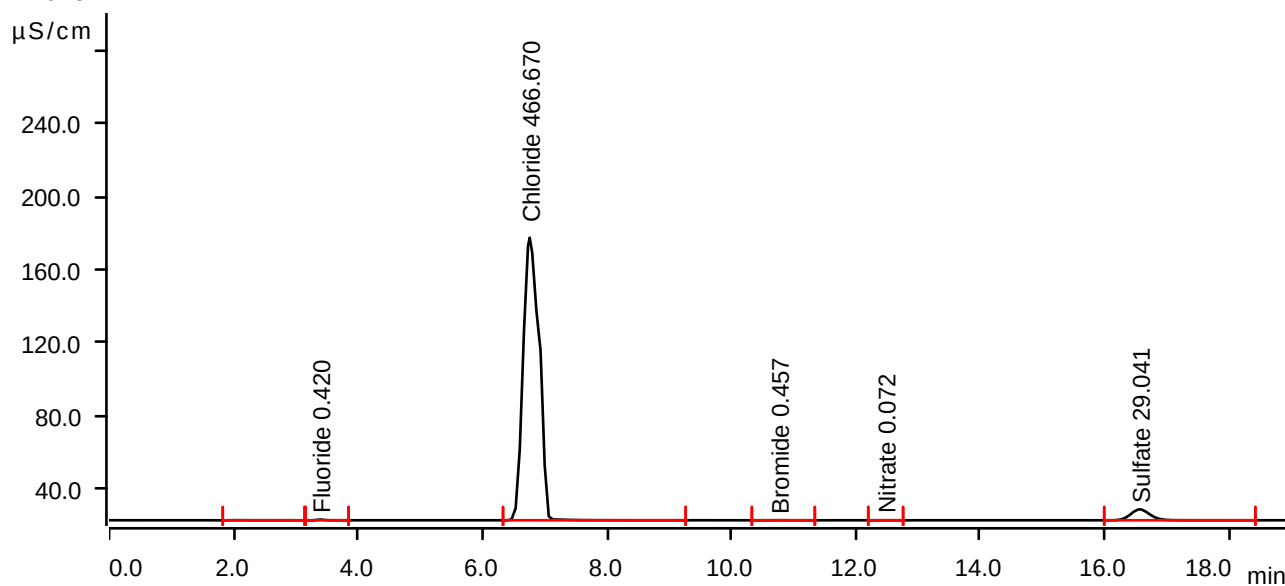

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	2.072	0.0504	0.091	invalid	
2	3.392	0.0555	0.425	0.420	Fluoride
3	6.760	45.8972	154.488	466.670	Chloride
4	10.762	0.0101	0.043	0.457	Bromide
5	12.475	0.0042	0.017	0.072	Nitrate
6	16.562	2.1650	5.991	29.041	Sulfate


Sample data

Ident P2718-02
Sample type Sample
Determination start 2024-06-04 19:46:19 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.04 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

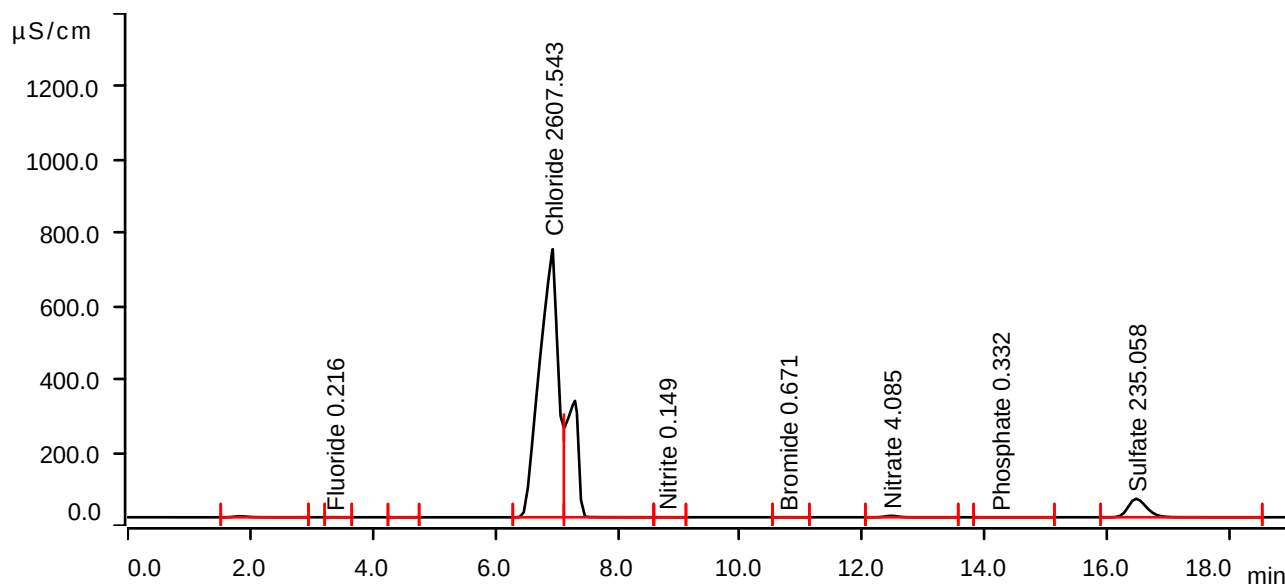

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.835	0.7880	2.870	invalid	
2	3.373	0.0259	0.184	0.216	Fluoride
3	4.563	0.0038	0.018	invalid	
4	6.940	256.4750	732.756	2607.543	Chloride
5	7.303	72.4679	318.202	invalid	
6	8.795	0.0107	0.061	0.149	Nitrite
7	10.773	0.0195	0.092	0.671	Bromide
8	12.463	0.9987	4.033	4.085	Nitrate
9	14.238	0.0172	0.045	0.332	Phosphate
10	16.465	17.8068	50.668	235.058	Sulfate


Sample data

Ident P2718-03
Sample type Sample
Determination start 2024-06-04 20:07:51 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.98 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

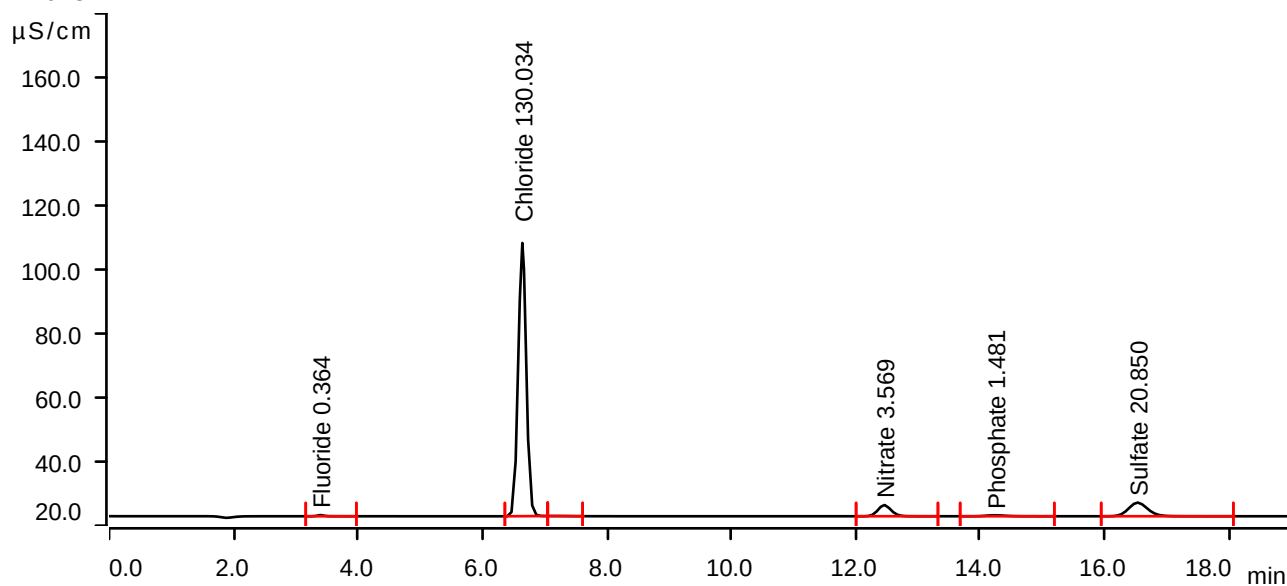

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.0473	0.372	0.364	Fluoride
2	6.642	12.7854	85.343	130.034	Chloride
3	7.182	0.0056	0.018	invalid	
4	12.457	0.8708	3.486	3.569	Nitrate
5	14.238	0.1153	0.310	1.481	Phosphate
6	16.528	1.5432	4.256	20.850	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-06-04 20:29:23 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

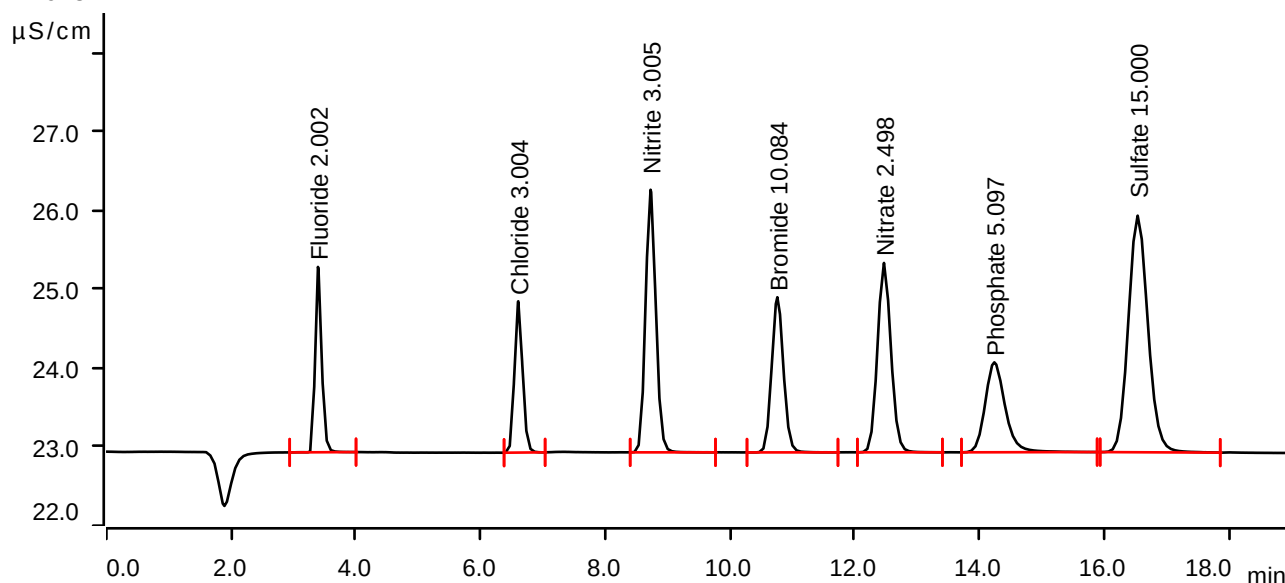

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.2858	2.352	2.002	Fluoride
2	6.605	0.2906	1.920	3.004	Chloride
3	8.725	0.6404	3.332	3.005	Nitrite
4	10.758	0.4336	1.969	10.084	Bromide
5	12.467	0.6052	2.403	2.498	Nitrate
6	14.237	0.4242	1.141	5.097	Phosphate
7	16.535	1.0990	3.002	15.000	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-06-04 20:50:52 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.78 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

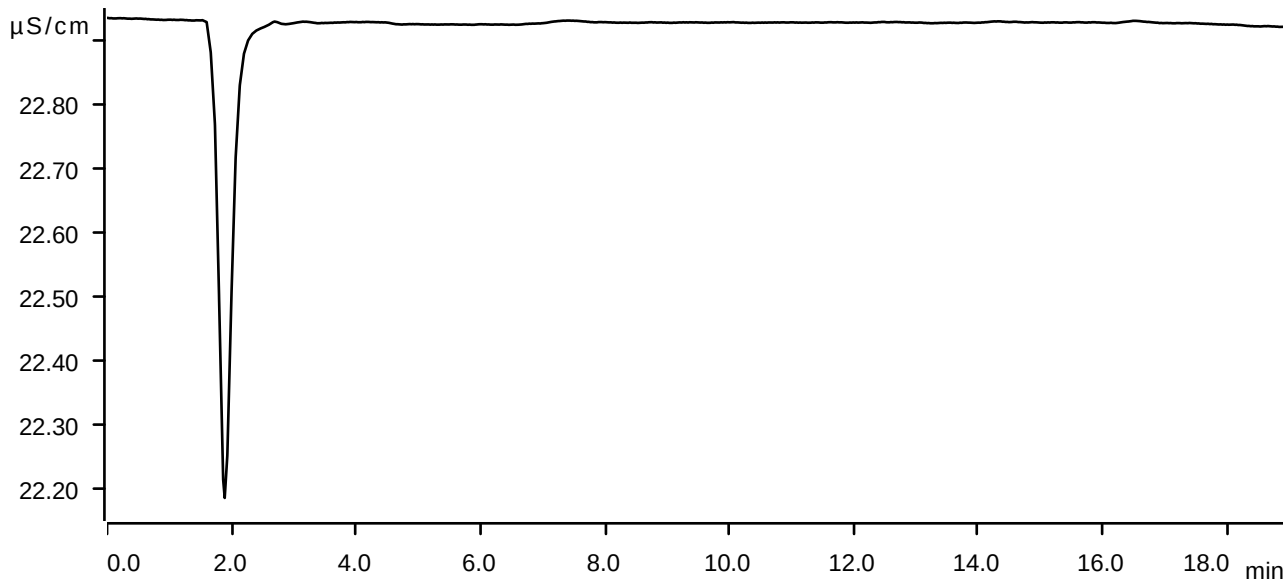


Sample data

Ident P2718-04
Sample type Sample
Determination start 2024-06-04 21:12:21 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

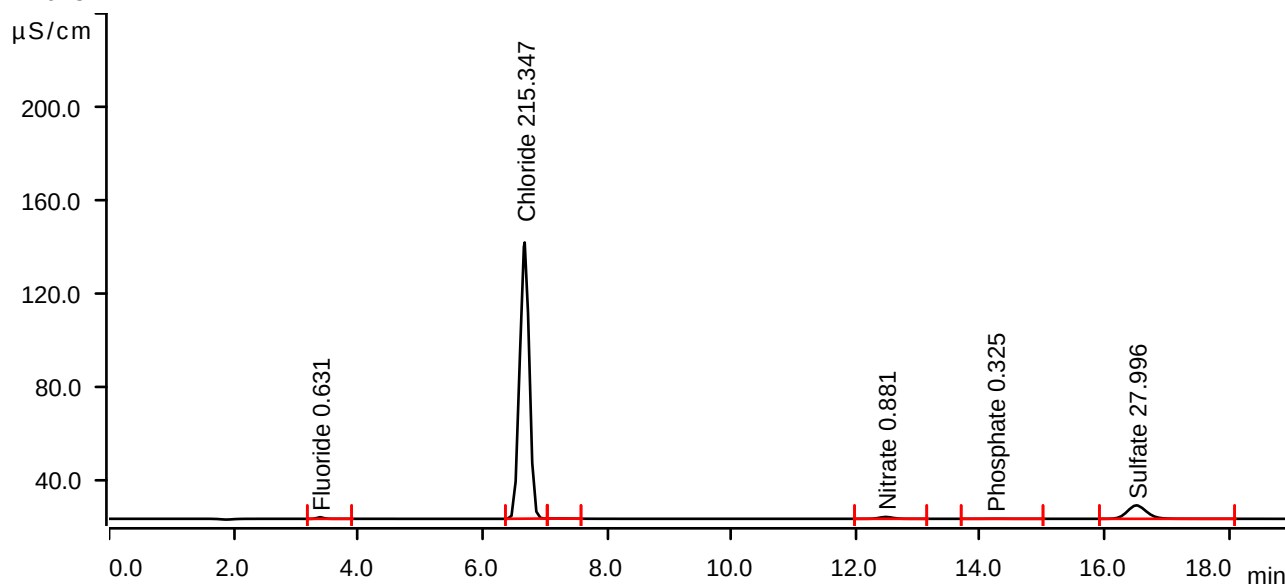

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.388	0.0862	0.692	0.631	Fluoride
2	6.680	21.1769	118.641	215.347	Chloride
3	7.157	0.0113	0.037	invalid	
4	12.482	0.2046	0.807	0.881	Nitrate
5	14.237	0.0166	0.043	0.325	Phosphate
6	16.508	2.0857	5.774	27.996	Sulfate


Sample data

Ident P2718-05
Sample type Sample
Determination start 2024-06-04 21:33:52 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

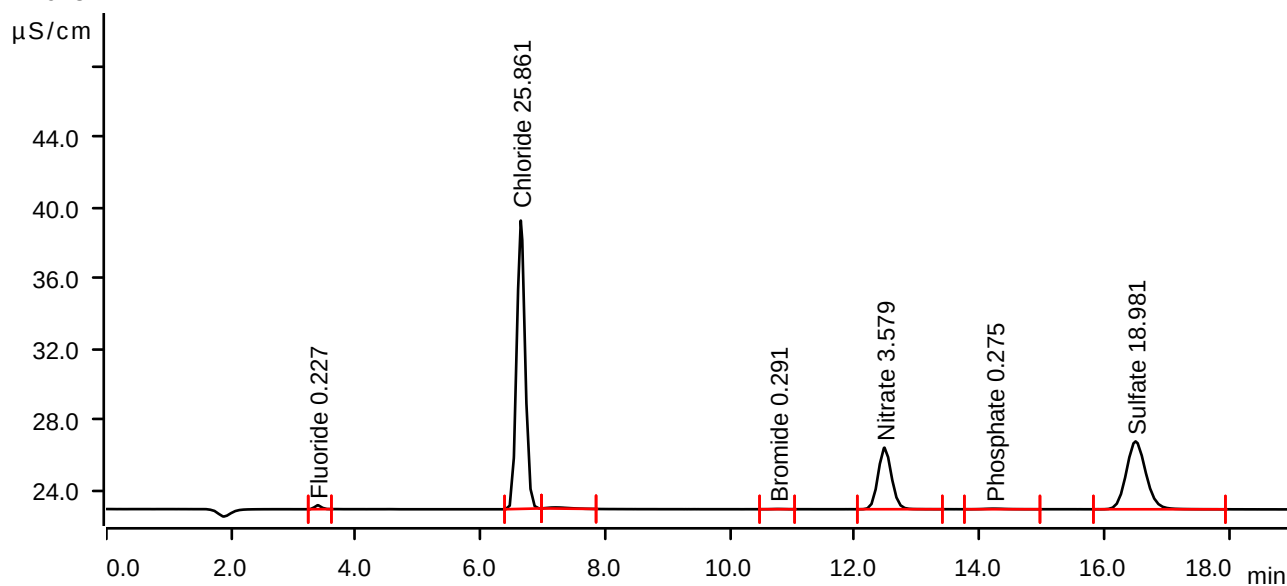

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.387	0.0274	0.226	0.227	Fluoride
2	6.645	2.5388	16.323	25.861	Chloride
3	7.207	0.0242	0.063	invalid	
4	10.763	0.0028	0.013	0.291	Bromide
5	12.477	0.8734	3.485	3.579	Nitrate
6	14.230	0.0124	0.032	0.275	Phosphate
7	16.502	1.4012	3.843	18.981	Sulfate


Sample data

Ident CCV
Sample type Sample
Determination start 2024-06-04 21:55:22 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

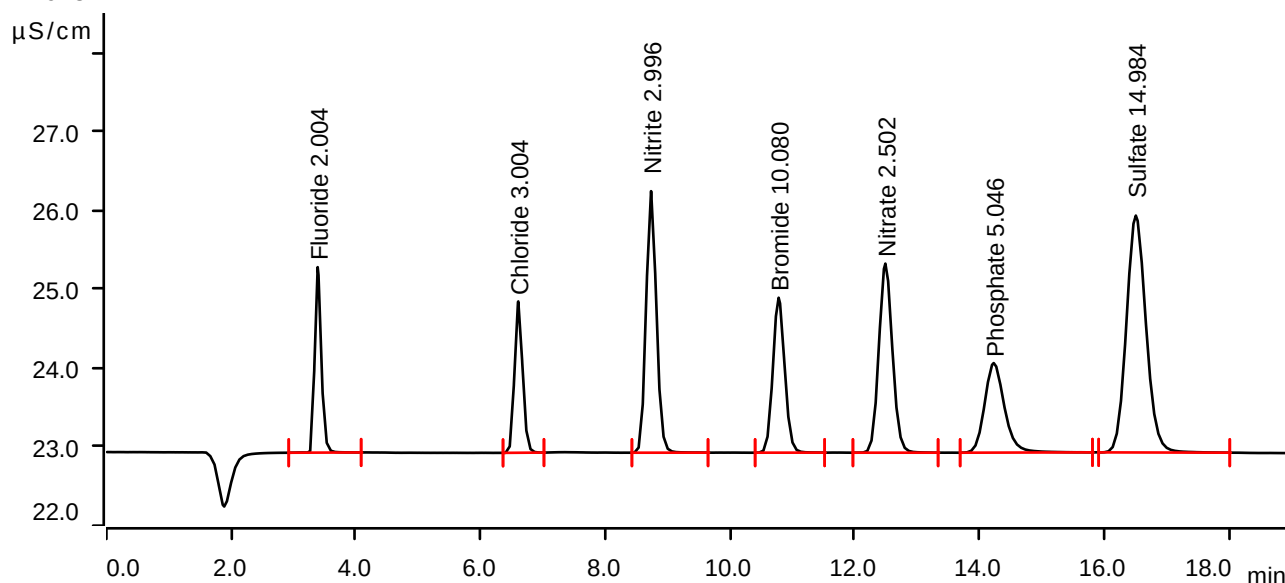

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.388	0.2861	2.354	2.004	Fluoride
2	6.605	0.2906	1.920	3.004	Chloride
3	8.733	0.6385	3.319	2.996	Nitrite
4	10.778	0.4335	1.966	10.080	Bromide
5	12.490	0.6065	2.400	2.502	Nitrate
6	14.227	0.4199	1.137	5.046	Phosphate
7	16.505	1.0978	3.006	14.984	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-06-04 22:16:51 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.67 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

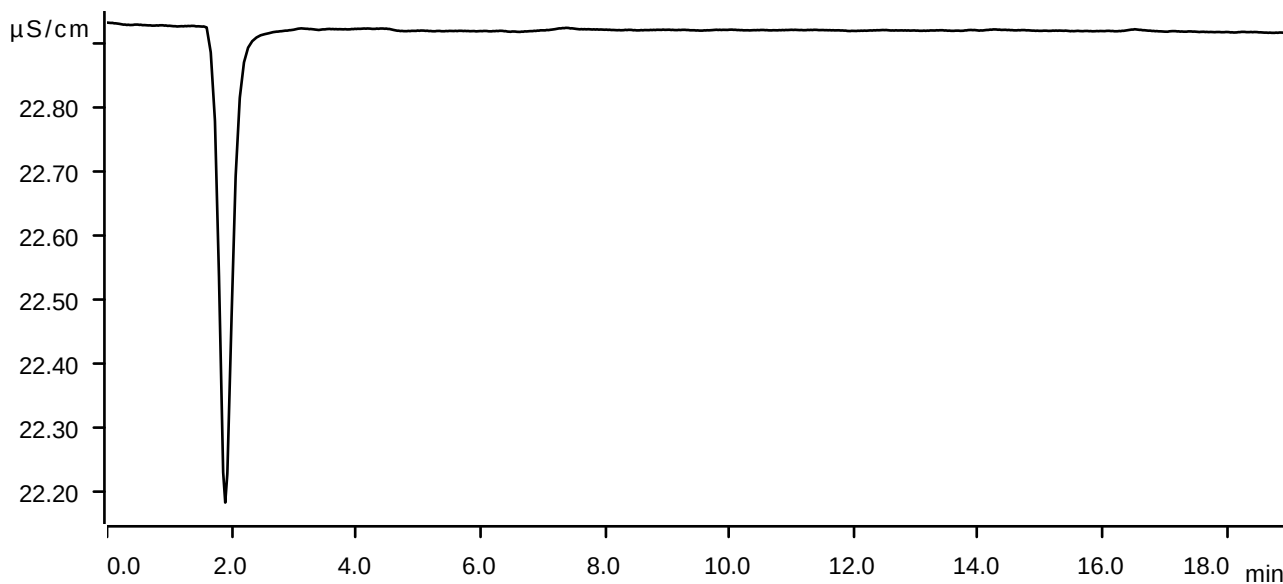


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-06-05 11:17:01 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

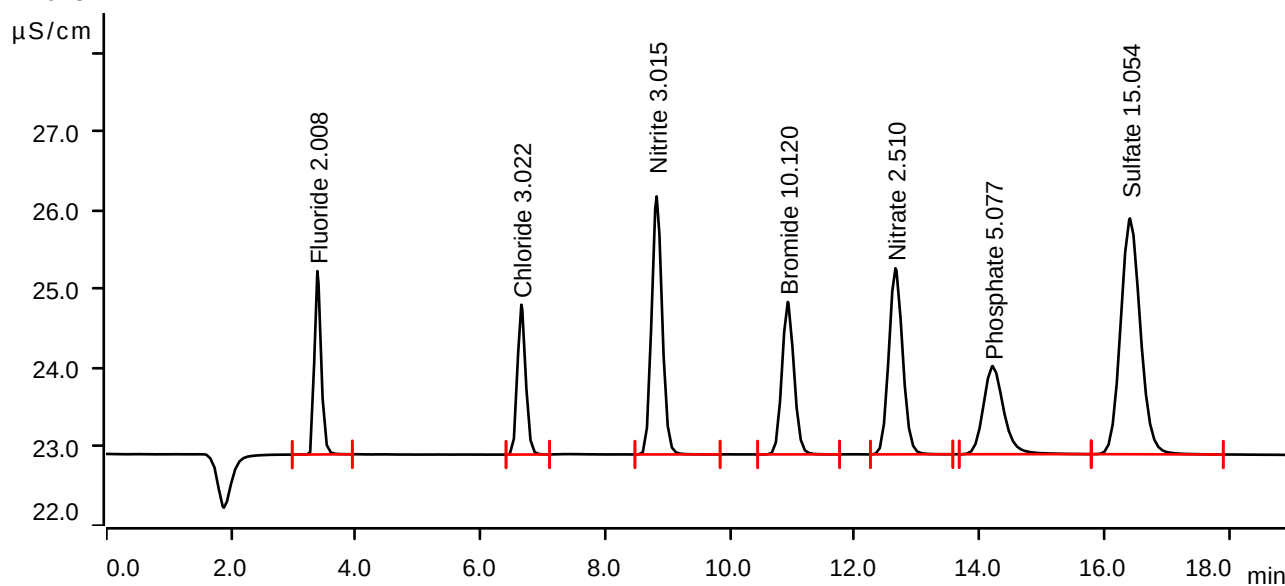

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.383	0.2866	2.327	2.008	Fluoride
2	6.653	0.2923	1.902	3.022	Chloride
3	8.823	0.6425	3.275	3.015	Nitrite
4	10.925	0.4352	1.935	10.120	Bromide
5	12.652	0.6082	2.362	2.510	Nitrate
6	14.210	0.4226	1.118	5.077	Phosphate
7	16.412	1.1031	2.993	15.054	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-06-05 11:38:32 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

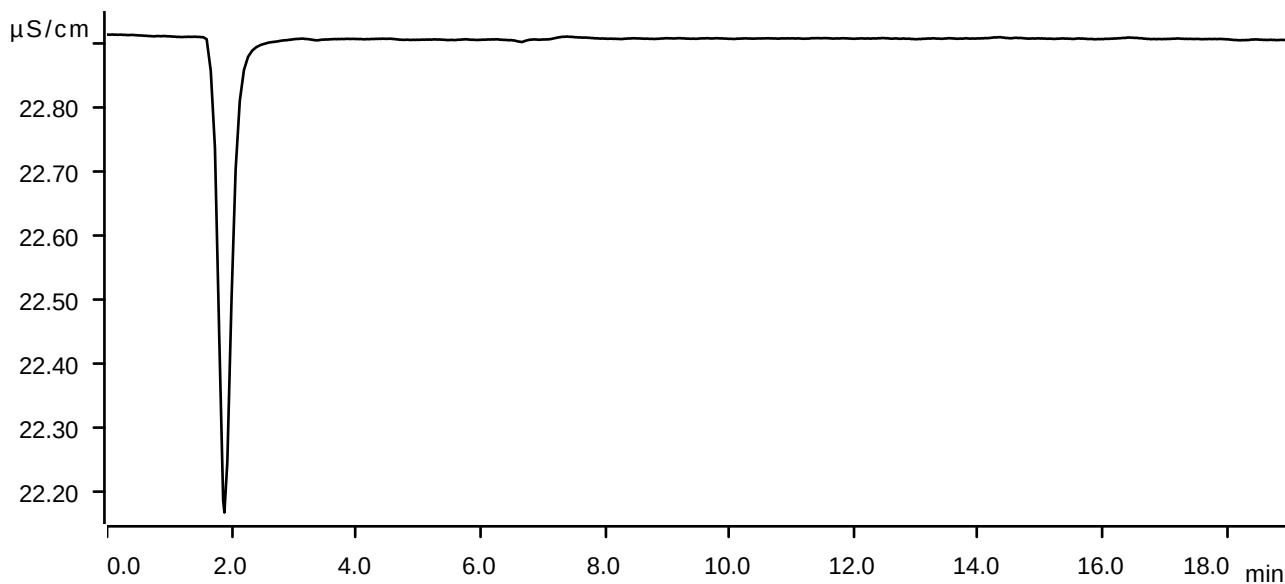


Sample data

Ident LB131061BLW2
Sample type Sample
Determination start 2024-06-05 12:00:02 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

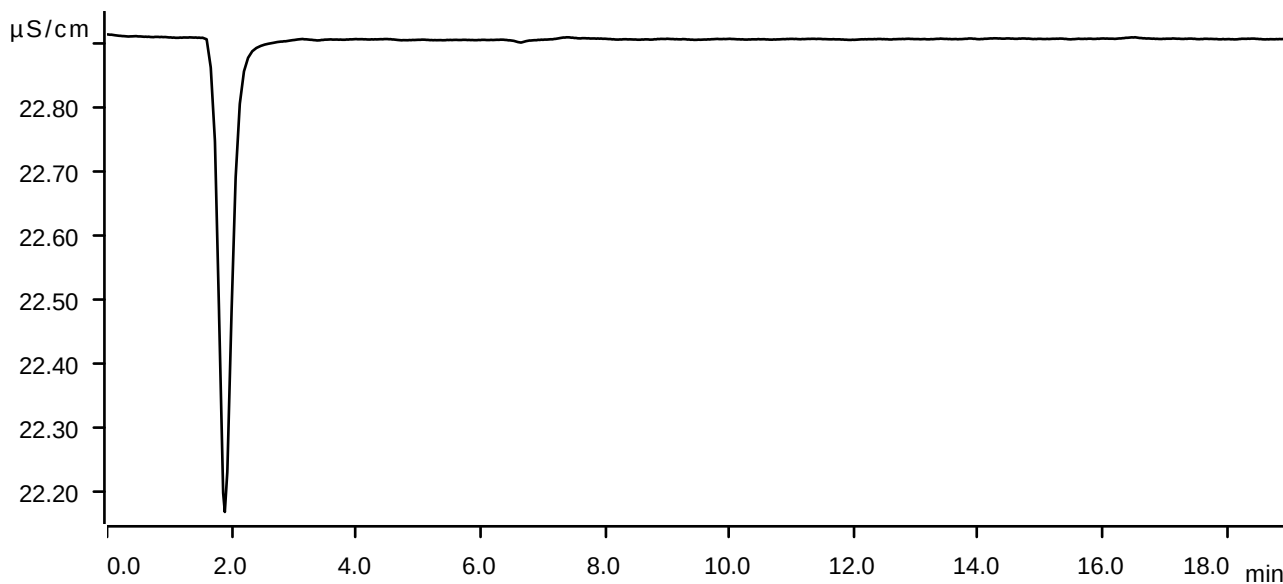


Sample data

Ident LB131061BSW2
Sample type Check standard 1
Determination start 2024-06-05 12:21:32 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

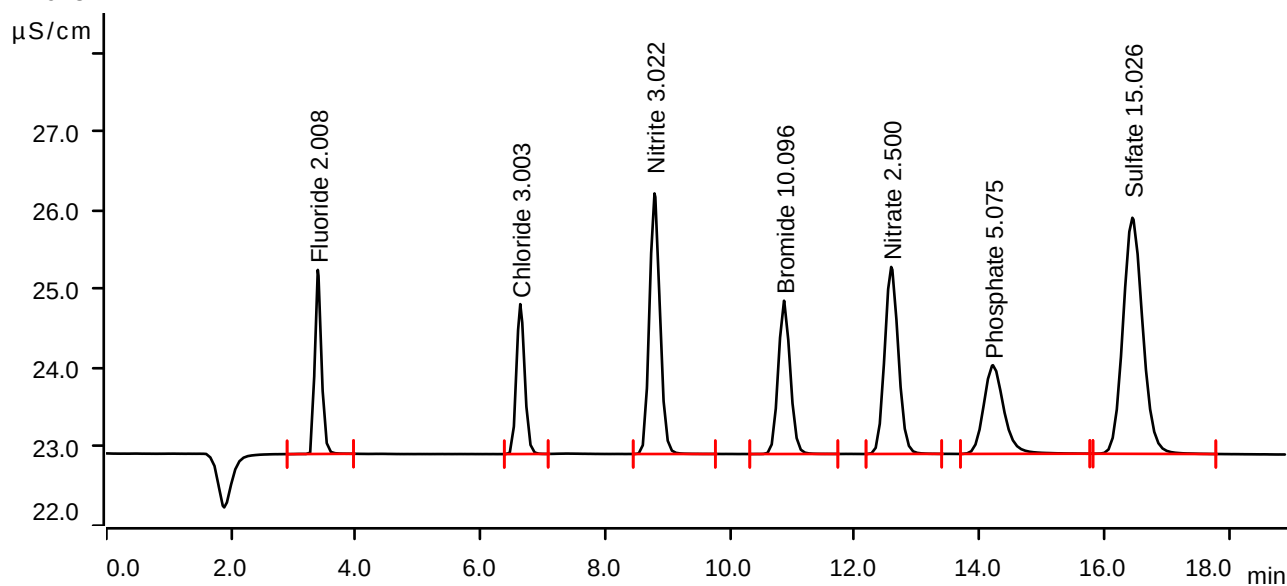

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.2867	2.336	2.008	Fluoride
2	6.637	0.2905	1.903	3.003	Chloride
3	8.788	0.6442	3.307	3.022	Nitrite
4	10.865	0.4342	1.945	10.096	Bromide
5	12.583	0.6059	2.373	2.500	Nitrate
6	14.215	0.4224	1.125	5.075	Phosphate
7	16.450	1.1010	2.996	15.026	Sulfate


Sample data

Ident P2717-01DLX5
Sample type Sample
Determination start 2024-06-05 12:43:04 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

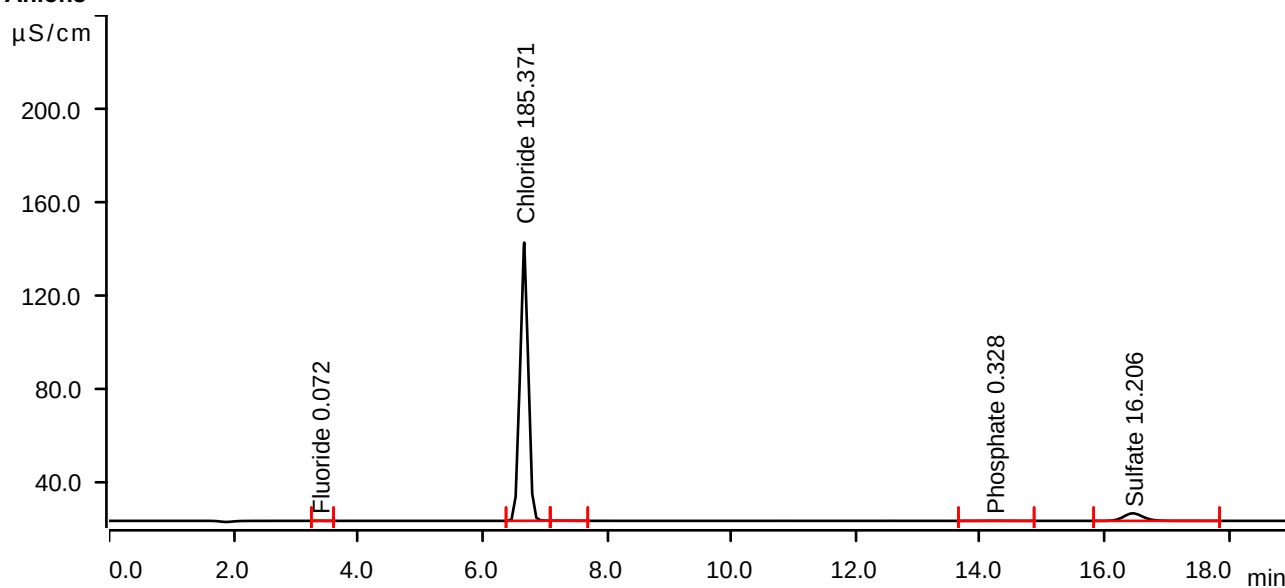

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.382	0.0049	0.041	0.072	Fluoride
2	6.673	18.2283	119.513	185.371	Chloride
3	7.225	0.0058	0.017	invalid	
4	14.225	0.0169	0.045	0.328	Phosphate
5	16.452	1.1905	3.252	16.206	Sulfate


Sample data

Ident P2717-02DLX10
Sample type Sample
Determination start 2024-06-05 13:04:38 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

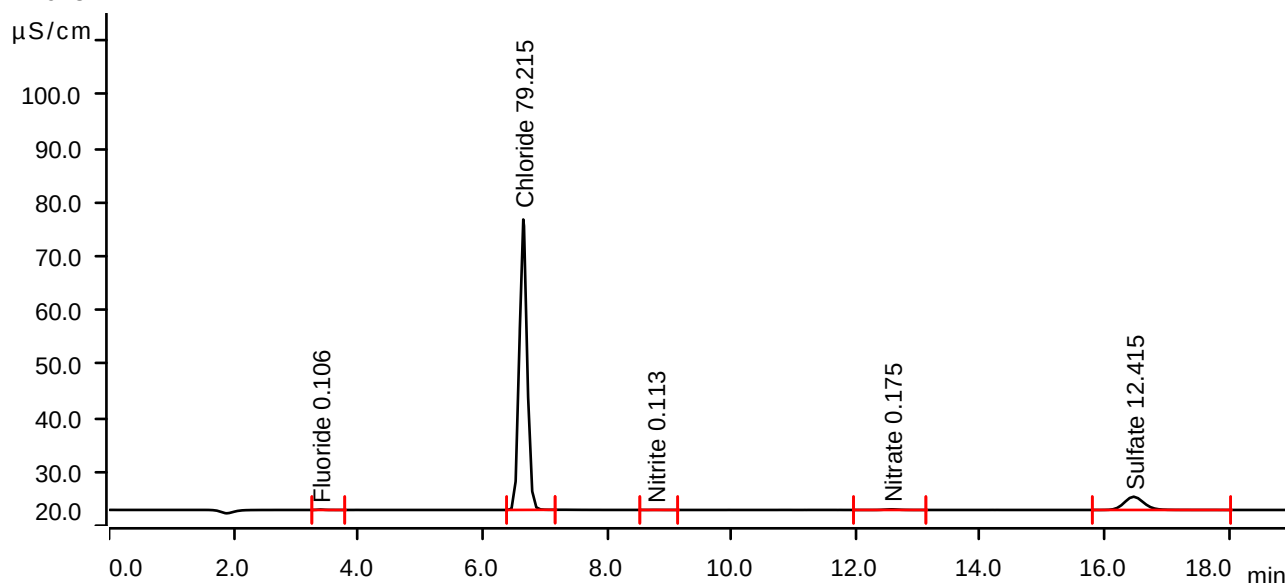

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.393	0.0097	0.078	0.106	Fluoride
2	6.657	7.7867	53.862	79.215	Chloride
3	8.775	0.0028	0.014	0.113	Nitrite
4	12.577	0.0296	0.114	0.175	Nitrate
5	16.465	0.9027	2.456	12.415	Sulfate


Sample data

Ident P2717-03DLX5
Sample type Sample
Determination start 2024-06-05 13:26:13 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

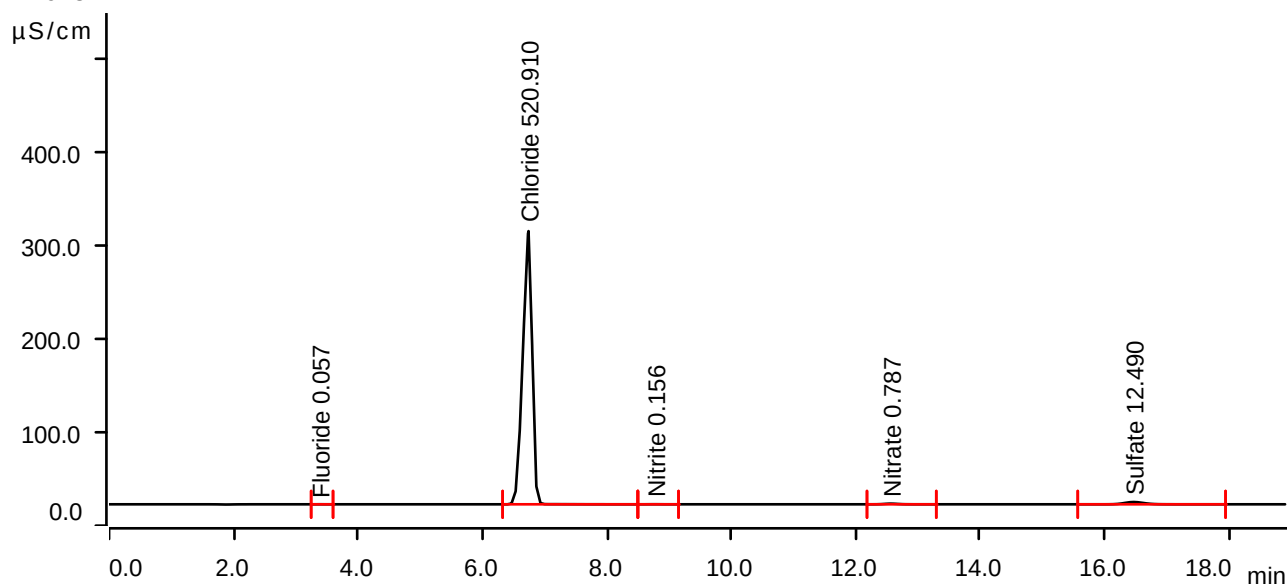

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.382	0.0027	0.022	0.057	Fluoride
2	6.742	51.2322	293.355	520.910	Chloride
3	8.775	0.0122	0.063	0.156	Nitrite
4	12.562	0.1812	0.707	0.787	Nitrate
5	16.465	0.9084	2.472	12.490	Sulfate


Sample data

Ident P2718-02DLX10
Sample type Sample
Determination start 2024-06-05 13:47:47 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

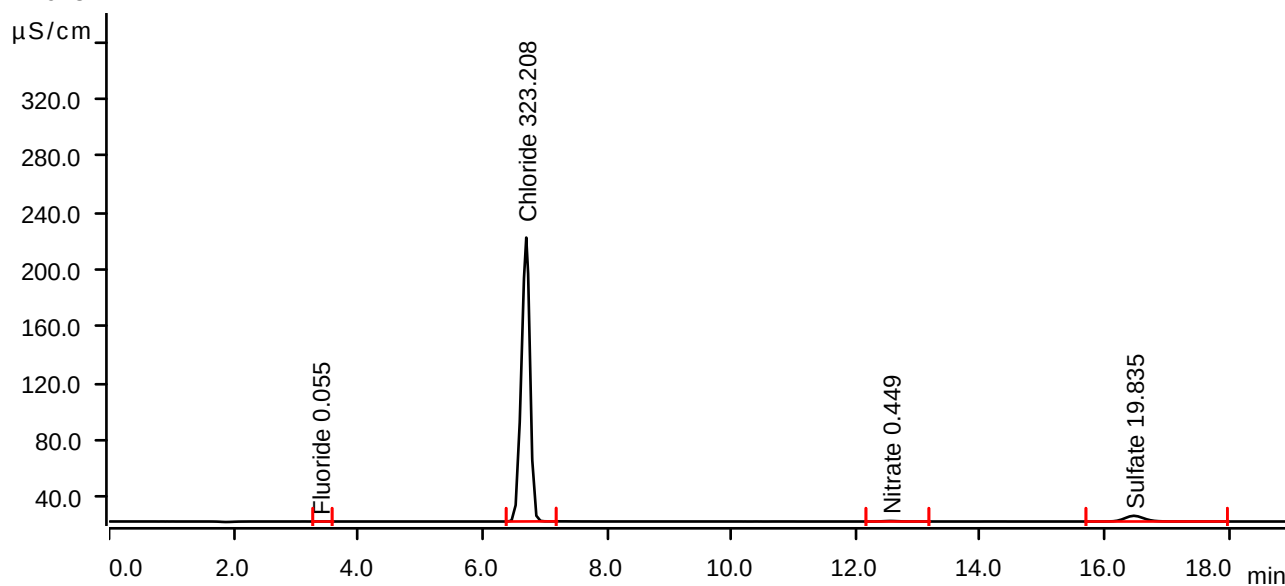

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.0024	0.020	0.055	Fluoride
2	6.705	31.7861	199.505	323.208	Chloride
3	12.557	0.0975	0.380	0.449	Nitrate
4	16.468	1.4661	4.022	19.835	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-06-05 14:09:21 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

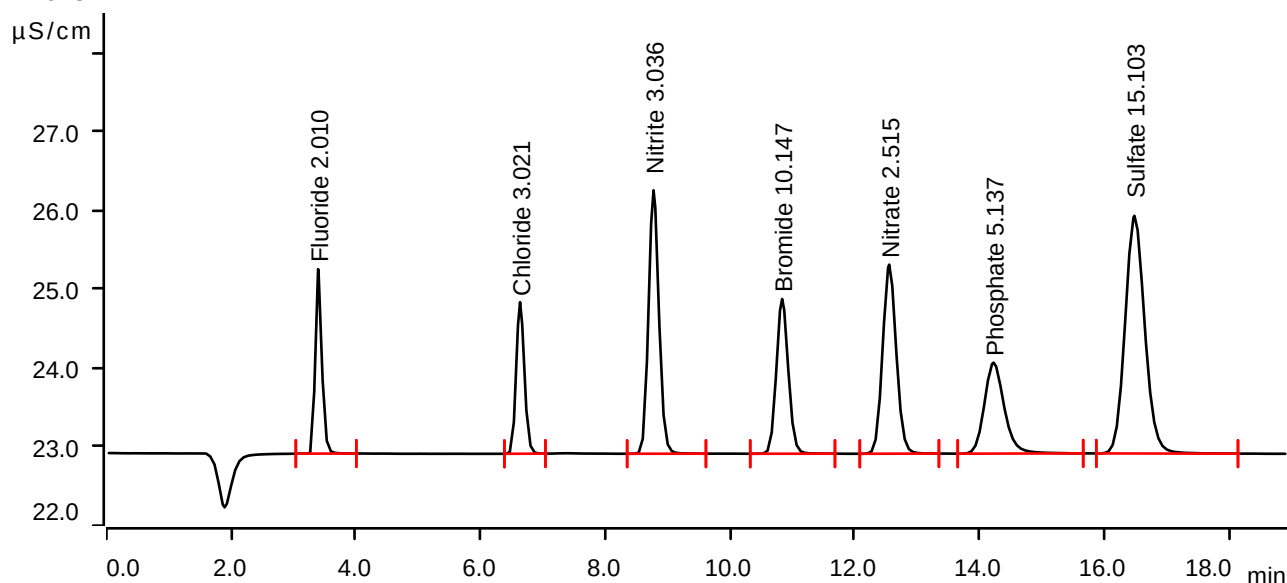

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.395	0.2870	2.341	2.010	Fluoride
2	6.633	0.2923	1.923	3.021	Chloride
3	8.773	0.6472	3.343	3.036	Nitrite
4	10.835	0.4364	1.964	10.147	Bromide
5	12.552	0.6095	2.399	2.515	Nitrate
6	14.225	0.4277	1.155	5.137	Phosphate
7	16.483	1.1068	3.017	15.103	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-06-05 14:30:51 UTC-4
Method IC1-051324
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

