


LB131189

SFAM01.1

INSTRUMENT ID: CV1

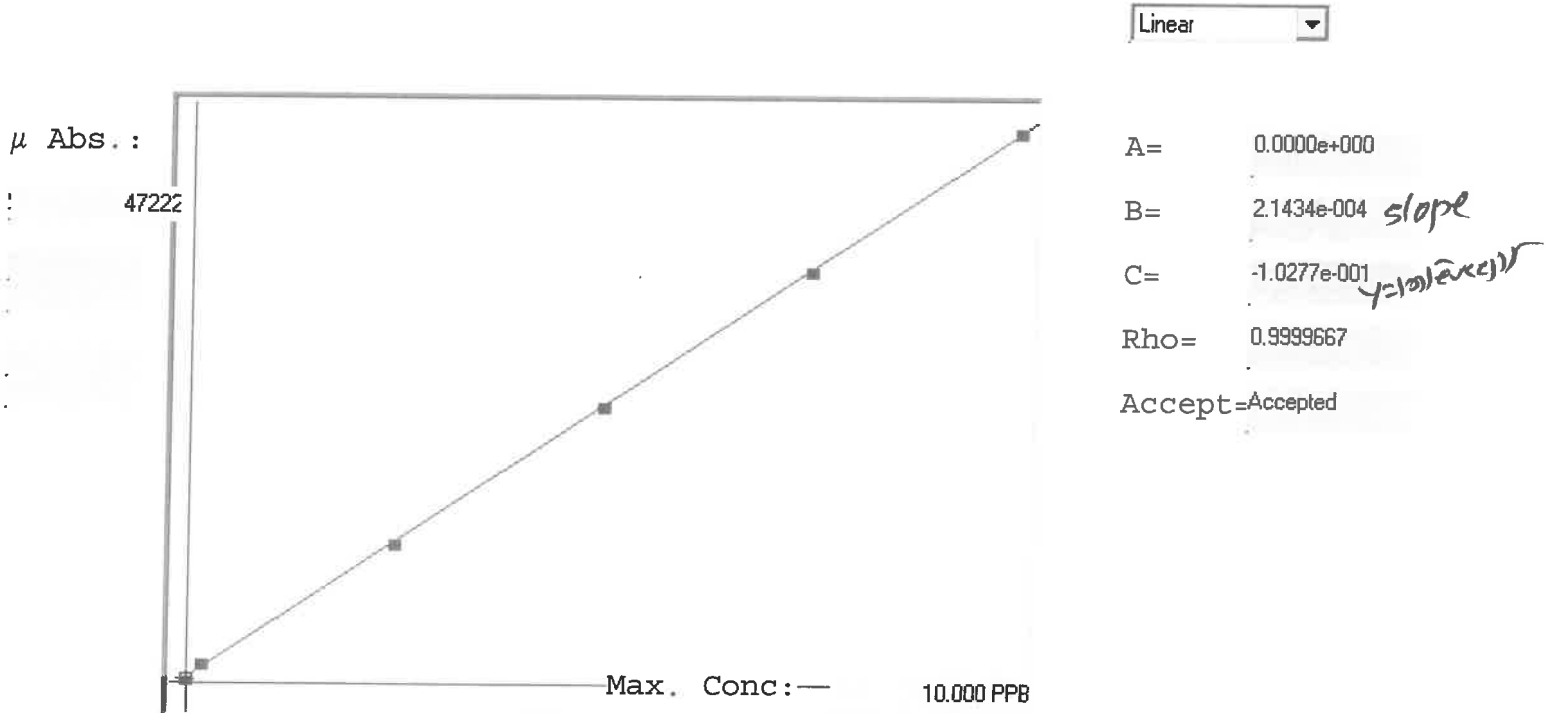

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	<i>a/d</i>
0.00	0.000	-0.024	-0.024	367	0.000	367					0
0.05	0.050					442	0				11
0.20	0.200	0.253	0.053	1658	0.0 %	1658					27
2.50	2.500	2.465	-0.035	11982	0.0 %	11982					1
5.00	5.000	5.009	0.009	23848	0.0 %	23848					0
7.50	7.500	7.478	-0.022	35370	0.0 %	35370					0
10.0	10.000	10.019	0.019	47222	0.0 %	47222					0

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	367	-		0 SFAM01.1	PPB	6/12/2024 10:20	Std
	0.2 S01	1658	-		0.2 SFAM01.1	PPB	6/12/2024 10:22	Std
	2.5 S02	11982	-		2.5 SFAM01.1	PPB	6/12/2024 10:25	Std
	5 S03	23848	-		5 SFAM01.1	PPB	6/12/2024 10:27	Std
	7.5 S04	35370	-		7.5 SFAM01.1	PPB	6/12/2024 10:29	Std
	10 S05	47222	-		10 SFAM01.1	PPB	6/12/2024 10:32	Std
ICV084	ICV084	19363	4.0475 -		SFAM01.1	PPB	6/12/2024 10:34	SMPL
ICB084	ICB084	419	-0.013 -		SFAM01.1	PPB	6/12/2024 10:39	SMPL
CCV021	CCV021	24118	5.0667 -		SFAM01.1	PPB	6/12/2024 10:42	SMPL
CCB021	CCB021	535	0.0119 -		SFAM01.1	PPB	6/12/2024 10:44	SMPL
PB161453BL	PBS453	275	-0.0438 -		SFAM01.1	PPB	6/12/2024 10:49	SMPL
P2643-01	MA4C18	9054	1.8379 -		SFAM01.1	PPB	6/12/2024 10:51	SMPL
P2643-02	MA4C18D	9020	1.8306 -		SFAM01.1	PPB	6/12/2024 10:53	SMPL
P2643-03	MA4C18S	21130	4.4262 -		SFAM01.1	PPB	6/12/2024 10:55	SMPL
P2643-04	MA4BH0	2402	0.4121 -		SFAM01.1	PPB	6/12/2024 10:58	SMPL
P2643-05	MA4BH1	6988	1.395 -		SFAM01.1	PPB	6/12/2024 11:00	SMPL
P2643-06	MA4BH2	565	0.0183 -		SFAM01.1	PPB	6/12/2024 11:02	SMPL
P2643-07	MA4BH3	143	-0.0721 -		SFAM01.1	PPB	6/12/2024 11:05	SMPL
P2643-08	MA4BH6	4800	0.9261 -		SFAM01.1	PPB	6/12/2024 11:07	SMPL
P2643-11	MA4B32	8417	1.7013 -		SFAM01.1	PPB	6/12/2024 11:09	SMPL
P2643-12	MA4B35	8872	1.7989 -		SFAM01.1	PPB	6/12/2024 11:11	SMPL
P2643-13	MA4B36	5121	0.9949 -		SFAM01.1	PPB	6/12/2024 11:14	SMPL
P2643-14	MA4B37	1934	0.3118 -		SFAM01.1	PPB	6/12/2024 11:16	SMPL
P2643-15	MA4BH7	9594	1.9536 -		SFAM01.1	PPB	6/12/2024 11:18	SMPL
P2643-16	MA4BH8	1395	0.1962 -		SFAM01.1	PPB	6/12/2024 11:20	SMPL
P2643-17	MA4BJ0	11847	2.4365 -		SFAM01.1	PPB	6/12/2024 11:23	SMPL
P2643-18	MA4BJ1	15842	3.2928 -		SFAM01.1	PPB	6/12/2024 11:25	SMPL
P2643-19	MA4BJ7	10245	2.0931 -		SFAM01.1	PPB	6/12/2024 11:27	SMPL
P2643-20	MA4BJ8	8649	1.7511 -		SFAM01.1	PPB	6/12/2024 11:30	SMPL
P2643-21	MA4BK5	21745	4.5581 -		SFAM01.1	PPB	6/12/2024 11:32	SMPL
CCV022	CCV022	24253	5.0956 -		SFAM01.1	PPB	6/12/2024 11:34	SMPL
CCB022	CCB022	681	0.0432 -		SFAM01.1	PPB	6/12/2024 11:36	SMPL
P2643-22	MA4BL3	6217	1.2298 -		SFAM01.1	PPB	6/12/2024 11:39	SMPL
PB161454BL	PBS454	404	-0.0162 -		SFAM01.1	PPB	6/12/2024 11:44	SMPL
P2649-01	MBH5T4	32530	6.8697 -		SFAM01.1	PPB	6/12/2024 11:46	SMPL
P2649-02	MBH5T5	25913	5.4514 -		SFAM01.1	PPB	6/12/2024 11:48	SMPL
P2649-03	MBH5T5D	22474	4.7143 -		SFAM01.1	PPB	6/12/2024 11:51	SMPL
P2649-04	MBH5T5S	37367	7.9065 -		SFAM01.1	PPB	6/12/2024 11:56	SMPL
P2649-05	MBH5T6	10849	2.2226 -		SFAM01.1	PPB	6/12/2024 11:58	SMPL
P2649-06	MBH5T7	2929	0.525 -		SFAM01.1	PPB	6/12/2024 12:01	SMPL
P2649-07	MBHBS1	15628	3.2469 -		SFAM01.1	PPB	6/12/2024 12:03	SMPL
P2649-08	MBHBS2	24305	5.1068 -		SFAM01.1	PPB	6/12/2024 12:05	SMPL
P2649-09	MBHBS3	22161	4.6472 -		SFAM01.1	PPB	6/12/2024 12:08	SMPL
P2649-10	MBHBS4	20308	4.25 -		SFAM01.1	PPB	6/12/2024 12:10	SMPL
P2649-11	MBHBS5	5904	1.1627 -		SFAM01.1	PPB	6/12/2024 12:12	SMPL
P2649-12	MBHBS6	18358	3.8321 -		SFAM01.1	PPB	6/12/2024 12:14	SMPL

LB131189

INSTRUMENT ID : CV1

P2649-13	MBHBS7	20877	4.372 -	SFAM01.1	PPB	6/12/2024 12:17 SMPL
P2649-14	MBHBS8	19637	4.1062 -	SFAM01.1	PPB	6/12/2024 12:19 SMPL
P2649-15	MBHBS9	23435	4.9203 -	SFAM01.1	PPB	6/12/2024 12:21 SMPL
P2649-16	MBHBT0	16077	3.3432 -	SFAM01.1	PPB	6/12/2024 12:24 SMPL
P2649-17	MBHBT1	15258	3.1676 -	SFAM01.1	PPB	6/12/2024 12:26 SMPL
P2649-18	MBHBT2	23411	4.9151 -	SFAM01.1	PPB	6/12/2024 12:28 SMPL
CCV023	CCV023	24109	5.0648 -	SFAM01.1	PPB	6/12/2024 12:30 SMPL
CCB023	CCB023	233	-0.0528 -	SFAM01.1	PPB	6/12/2024 12:33 SMPL
P2649-19	MBHBT3	17012	3.5436 -	SFAM01.1	PPB	6/12/2024 12:35 SMPL
P2649-20	MBHBT4	7572	1.5202 -	SFAM01.1	PPB	6/12/2024 12:37 SMPL
P2649-21	MBHBT5	2883	0.5152 -	SFAM01.1	PPB	6/12/2024 12:40 SMPL
P2649-22	MBHBT6	13707	2.8352 -	SFAM01.1	PPB	6/12/2024 12:42 SMPL
CCV024	CCV024	24069	5.0562 -	SFAM01.1	PPB	6/12/2024 12:44 SMPL
CCB024	CCB024	227	-0.0541 -	SFAM01.1	PPB	6/12/2024 12:46 SMPL