


LB131401

7471B

INSTRUMENT ID? CV4

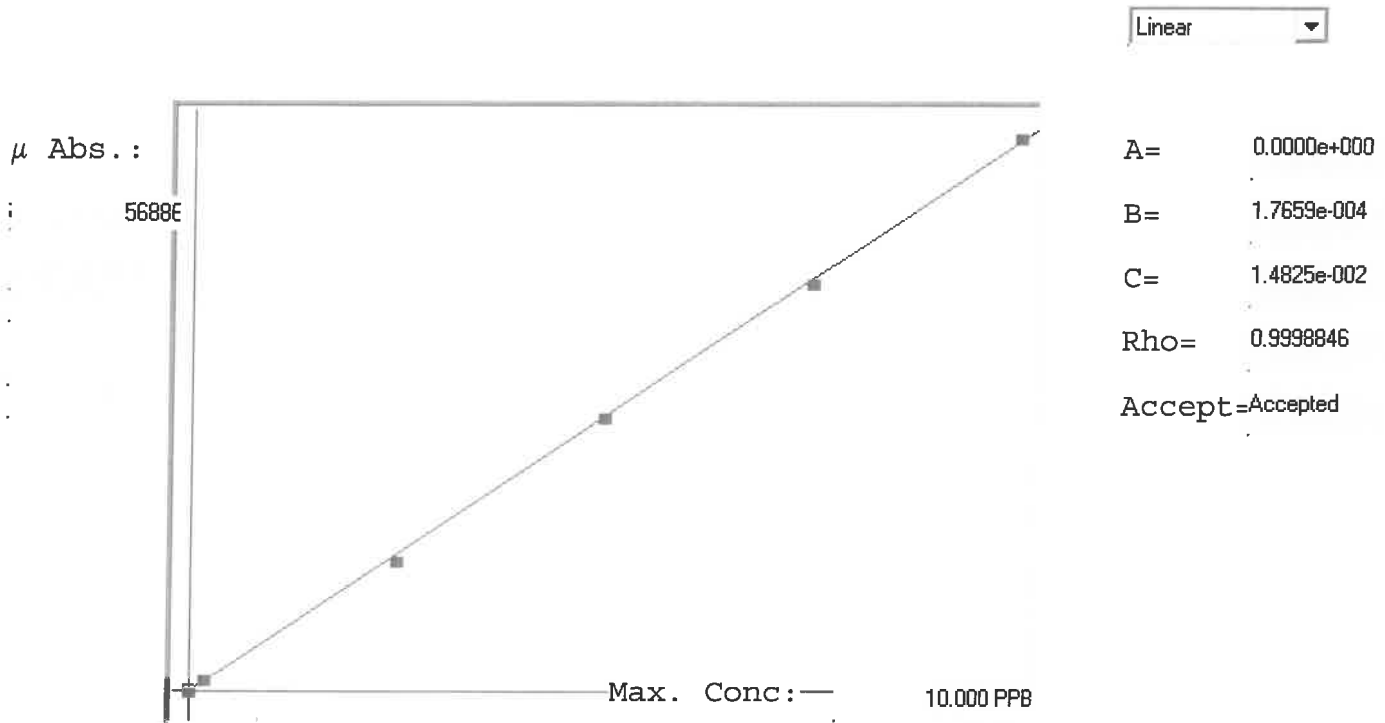

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	6/11
0.0	0.000	0.047	0.047	184	0.000	184					
0.2	0.200	0.236	0.036	1251	0.0 %	1251					
2.5	2.500	2.408	-0.092	13553	0.0 %	13553					
5.0	5.000	5.005	0.005	28260	0.0 %	28260					
7.5	7.500	7.443	-0.057	42065	0.0 %	42065					
10.0	10.000	10.060	0.060	56886	0.0 %	56886					

LB131401 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 25 Jun 2024 10:29:12

Sample ID	Extended ID	µ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	184	-	0.0000	7471B	PPB	25 Jun 2024 10:29:26	S	Std
0.2 - 1	50.2	1251	-	0.2000	7471B	PPB	25 Jun 2024 10:31:44	S	Std
2.5 - 1	52.5	13553	-	2.5000	7471B	PPB	25 Jun 2024 10:34:02	S	Std
5.0 - 1	55	28260	-	5.0000	7471B	PPB	25 Jun 2024 10:36:20	S	Std
7.5 - 1	57.5	42065	-	7.5000	7471B	PPB	25 Jun 2024 10:38:38	S	Std
10.0 - 1	50	56886	-	10.0000	7471B	PPB	25 Jun 2024 10:43:39	S	Std
ICV04 - 1	ICV04	21898	3.8818	-	7471B	PPB	25 Jun 2024 10:46:25	U	SMPL
ICB04 - 1	ICB04	287	0.0655	-	7471B	PPB	25 Jun 2024 10:51:15	U	SMPL
CCV84 - 1	CCV84	28388	5.0279	-	7471B	PPB	25 Jun 2024 10:53:30	U	SMPL
CCB84 - 1	CCB84	-8	0.0134	-	7471B	PPB	25 Jun 2024 10:55:45	U	SMPL
CRA - 1	CRA	1243	0.2343	-	7471B	PPB	25 Jun 2024 10:58:04	U	SMPL
HighStd - 1	HighStd	56466	9.9862	-	7471B	PPB	25 Jun 2024 11:00:19	U	SMPL
ChkStd - 1	ChkStd	39403	6.9730	-	7471B	PPB	25 Jun 2024 11:02:34	U	SMPL
PB161689BL - 1	PBS	-18	0.0116	-	7471B	PPB	25 Jun 2024 11:04:56	U	SMPL
PB161689BS - 1	LCSS	22228	3.9401	-	7471B	PPB	25 Jun 2024 11:07:18	U	SMPL
P2977-01 - 1	OSTL-A1	4302	0.7745	-	7471B	PPB	25 Jun 2024 11:14:31	U	SMPL
P2977-01DUP - 1	OSTL-A1DUP	3861	0.6966	-	7471B	PPB	25 Jun 2024 11:16:47	U	SMPL
P2977-01MS - 1	OSTL-A1MS	25823	4.5749	-	7471B	PPB	25 Jun 2024 11:19:06	U	SMPL
P2977-01MSD - 1	OSTL-A1MSD	24771	4.3892	-	7471B	PPB	25 Jun 2024 11:21:23	U	SMPL
P2977-02 - 1	OSTL-A2	3407	0.6165	-	7471B	PPB	25 Jun 2024 11:23:41	U	SMPL
CCV85 - 1	CCV85	27969	4.9539	-	7471B	PPB	25 Jun 2024 11:25:59	U	SMPL
CCB85 - 1	CCB85	58	0.0251	-	7471B	PPB	25 Jun 2024 11:30:53	U	SMPL
P2977-03 - 1	OSTL-A3	4492	0.8081	-	7471B	PPB	25 Jun 2024 11:33:08	U	SMPL
P2977-04 - 1	OSTL-A4	4498	0.8091	-	7471B	PPB	25 Jun 2024 11:35:24	U	SMPL
P2977-05 - 1	OSTL-A5	2887	0.5246	-	7471B	PPB	25 Jun 2024 11:37:41	U	SMPL
P2977-06 - 1	OSTL-A6	3867	0.6977	-	7471B	PPB	25 Jun 2024 11:39:59	U	SMPL
P2977-07 - 1	OSTL-B1	3963	0.7147	-	7471B	PPB	25 Jun 2024 11:42:16	U	SMPL
P2977-08 - 1	OSTL-B2	4008	0.7226	-	7471B	PPB	25 Jun 2024 11:44:37	U	SMPL
P2977-09 - 1	OSTL-B3	4339	0.7811	-	7471B	PPB	25 Jun 2024 11:46:54	U	SMPL
P2977-10 - 1	OSTL-B4	4085	0.7362	-	7471B	PPB	25 Jun 2024 11:49:12	U	SMPL
P2977-11 - 1	OSTL-B5	5041	0.9050	-	7471B	PPB	25 Jun 2024 11:51:31	U	SMPL
P2977-12 - 1	OSTL-B6	3500	0.6329	-	7471B	PPB	25 Jun 2024 11:53:48	U	SMPL
CCV86 - 1	CCV86	28227	4.9995	-	7471B	PPB	25 Jun 2024 11:56:05	U	SMPL
CCB86 - 1	CCB86	-131	-0.0083	-	7471B	PPB	25 Jun 2024 11:58:22	U	SMPL
P2977-13 - 1	OSTL-C1	4186	0.7540	-	7471B	PPB	25 Jun 2024 12:00:41	U	SMPL
P2977-14 - 1	OSTL-C2	4036	0.7275	-	7471B	PPB	25 Jun 2024 12:02:56	U	SMPL
P2977-15 - 1	OSTL-C3	5165	0.9269	-	7471B	PPB	25 Jun 2024 12:05:14	U	SMPL
P2977-16 - 1	OSTL-C4	1682	0.3119	-	7471B	PPB	25 Jun 2024 12:07:32	U	SMPL
P2977-17 - 1	OSTL-C5	4064	0.7325	-	7471B	PPB	25 Jun 2024 12:09:50	U	SMPL
P2977-18 - 1	OSTL-C6	4102	0.7392	-	7471B	PPB	25 Jun 2024 12:12:08	U	SMPL
P2977-19 - 1	OSTL-D1	4134	0.7449	-	7471B	PPB	25 Jun 2024 12:14:25	U	SMPL
P2977-20 - 1	OSTL-D2	4088	0.7367	-	7471B	PPB	25 Jun 2024 12:16:42	U	SMPL
PB161690BL - 1	PBS	87	0.0302	-	7471B	PPB	25 Jun 2024 12:19:00	U	SMPL
PB161690BS - 1	LCSS	22331	3.9583	-	7471B	PPB	25 Jun 2024 12:21:17	U	SMPL
CCV87 - 1	CCV87	28197	4.9942	-	7471B	PPB	25 Jun 2024 12:23:33	U	SMPL
CCB87 - 1	CCB87	-149	-0.0115	-	7471B	PPB	25 Jun 2024 12:25:51	U	SMPL
P2977-21 - 1	OSTL-D3	6511	1.1646	-	7471B	PPB	25 Jun 2024 12:28:10	U	SMPL
P2977-22 - 1	OSTL-D4	3885	0.7009	-	7471B	PPB	25 Jun 2024 12:30:25	U	SMPL
P2977-23 - 1	OSTL-D5	4459	0.8022	-	7471B	PPB	25 Jun 2024 12:32:43	U	SMPL
P2977-24 - 1	OSTL-D6	3940	0.7106	-	7471B	PPB	25 Jun 2024 12:35:00	U	SMPL
P3008-01 - 1	WC-WS-6-21-24	39493	6.9889	-	7471B	PPB	25 Jun 2024 12:37:18	U	SMPL
P3009-01 - 1	VNJ-204	1274	0.2398	-	7471B	PPB	25 Jun 2024 12:39:36	U	SMPL
P3009-01DUP - 1	VNJ-204DUP	1498	0.2794	-	7471B	PPB	25 Jun 2024 12:41:55	U	SMPL
P3009-01MS - 1	VNJ-204MS	21873	3.8774	-	7471B	PPB	25 Jun 2024 12:44:12	U	SMPL
P3009-01MSD - 1	VNJ-204MSD	22217	3.9381	-	7471B	PPB	25 Jun 2024 12:46:29	U	SMPL
P3021-01 - 1	ARS20-008	59129	10.4565	-	7471B	PPB	25 Jun 2024 12:48:48	U	SMPL
CCV88 - 1	CCV88	27703	4.9069	-	7471B	PPB	25 Jun 2024 12:51:06	U	SMPL
CCB88 - 1	CCB88	-140	-0.0099	-	7471B	PPB	25 Jun 2024 12:53:29	U	SMPL
P3021-04 - 1	ARS20-0018	113694	20.0922	-	7471B	PPB	25 Jun 2024 12:55:48	U	SMPL
P3021-07 - 1	ARS20-006	79592	14.0700	-	7471B	PPB	25 Jun 2024 12:58:04	U	SMPL
P3021-10 - 1	ARS20-0015	75062	13.2701	-	7471B	PPB	25 Jun 2024 13:00:33	U	SMPL
P3022-01 - 1	BL-CONCRETE	1070	0.2038	-	7471B	PPB	25 Jun 2024 13:02:58	U	SMPL
P2977-01LX5 - 1		691	0.1368	-	7471B	PPB	25 Jun 2024 13:05:22	U	SMPL
P2977-01A - 1		25070	4.4420	-	7471B	PPB	25 Jun 2024 13:07:38	U	SMPL
P3009-01LX5 - 1		42	0.0222	-	7471B	PPB	25 Jun 2024 13:09:55	U	SMPL
P3009-01A - 1		22469	3.9826	-	7471B	PPB	25 Jun 2024 13:12:14	U	SMPL
CCV89 - 1	CCV89	28158	4.9873	-	7471B	PPB	25 Jun 2024 13:14:32	U	SMPL
CCB89 - 1	CCB89	-160	-0.0134	-	7471B	PPB	25 Jun 2024 13:16:50	U	SMPL
P3021-01DLX2 - 1		29295	5.1881	-	7471B	PPB	25 Jun 2024 13:19:10	U	SMPL
P3021-04DLX5 - 1		26288	4.6570	-	7471B	PPB	25 Jun 2024 13:21:27	U	SMPL
P3021-07DLX5 - 1		17789	3.1562	-	7471B	PPB	25 Jun 2024 13:23:46	U	SMPL
P3021-10DLX5 - 1		15593	2.7684	-	7471B	PPB	25 Jun 2024 13:26:06	U	SMPL
CCV90 - 1	CCV90	28087	4.9747	-	7471B	PPB	25 Jun 2024 13:28:24	U	SMPL
CCB90 - 1	CCB90	-181	-0.0171	-	7471B	PPB	25 Jun 2024 13:30:43	U	SMPL