

66131421

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

6/26/2024 15:47

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	96.012	0.0	0.087	
ICB001 ICB001	-0.357	0.0	0.001	
CCV001 CCV001	235.625	0.0	0.210	
CCB001 CCB001	0.126	0.0	0.001	
PB161749BL PBW749	0.520	0.0	0.002	
P3057-01 E08C7	0.218	0.0	0.002	
P3057-02 E08C7D	0.234	0.0	0.002	
P3057-03 E08C7S	107.752	0.0	0.097	
P3057-04 E08C9	0.916	0.0	0.002	
P3057-05 E08D4	1.098	0.0	0.002	
P3057-06 E08D7	-0.074	0.0	0.001	
P3082-01 E08E0	0.009	0.0	0.001	
P3082-02 E08E0D	-0.134	0.0	0.001	
P3082-03 E08E0S	97.075	0.0	0.087	
CCV002 CCV002	241.098	0.0	0.215	
CCB002 CCB002	0.108	0.0	0.001	

N 16
Mean 48.764
SD 84.0060
CV% 172.27

06/26/2024
RM

Aquakem v. 7.2AQ1

Results from time period:

Wed Jun 26 13:21:52 2024

Wed Jun 26 15:44:36 2024

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NEW	P	0.4585	µg/l	6/26/2024 13:21:52
S5.0	A	CNEPA-NEW	P	3.8833	µg/l	6/26/2024 13:21:53
S10.0	A	CNEPA-NEW	P	9.2592	µg/l	6/26/2024 13:21:54
S100.0	A	CNEPA-NEW	P	100.568	µg/l	6/26/2024 13:21:55
S250.0	A	CNEPA-NEW	P	251.8372	µg/l	6/26/2024 13:21:56
S500.0	A	CNEPA-NEW	P	498.9938	µg/l	6/26/2024 13:21:57
ICV001 ICV001	S	CNEPA-NEW	P	96.012	µg/l	6/26/2024 15:29:49
ICB001 ICB001	S	CNEPA-NEW	P	-0.3571	µg/l	6/26/2024 15:29:51
CCV001 CCV001	S	CNEPA-NEW	P	235.6246	µg/l	6/26/2024 15:29:52
CCB001 CCB001	S	CNEPA-NEW	P	0.1258	µg/l	6/26/2024 15:29:54
PB161749BL PBW749	S	CNEPA-NEW	P	0.5195	µg/l	6/26/2024 15:29:56
P3057-01 E08C7	S	CNEPA-NEW	P	0.2184	µg/l	6/26/2024 15:37:20
P3057-02 E08C7D	S	CNEPA-NEW	P	0.2338	µg/l	6/26/2024 15:37:22
P3057-03 E08C7S	S	CNEPA-NEW	P	107.752	µg/l	6/26/2024 15:37:23
P3057-04 E08C9	S	CNEPA-NEW	P	0.9161	µg/l	6/26/2024 15:37:25
P3057-05 E08D4	S	CNEPA-NEW	P	1.0981	µg/l	6/26/2024 15:37:26
P3057-06 E08D7	S	CNEPA-NEW	P	-0.074	µg/l	6/26/2024 15:37:27
P3082-01 E08E0	S	CNEPA-NEW	P	0.0086	µg/l	6/26/2024 15:37:30
P3082-02 E08E0D	S	CNEPA-NEW	P	-0.1339	µg/l	6/26/2024 15:44:27
P3082-03 E08E0S	S	CNEPA-NEW	P	97.0748	µg/l	6/26/2024 15:44:28
CCV002 CCV002	S	CNEPA-NEW	P	241.0976	µg/l	6/26/2024 15:44:32
CCB002 CCB002	S	CNEPA-NEW	P	0.1076	µg/l	6/26/2024 15:44:35

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

6/26/2024 13:49

Reviewed by : RM Instrument ID : Konelab

Test CNEPA-NEW


Accepted 6/26/2024 13:49

Factor- 1127 0.000888

Bias y Intercept 0.001 06/27/2024
RM

Coeff. of det. 0.999966

Errors

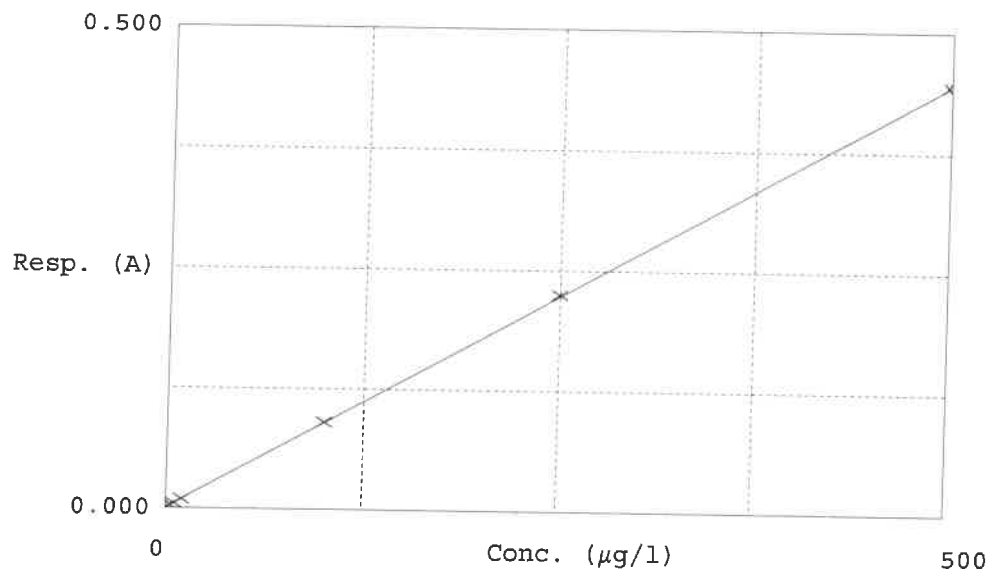

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCNS _{0.0}	0.002	0.4585	0.0000	-
2	5.0PPBCNS _{5.0}	0.005	3.8833	5.0000	-22.3
3	10PPBCNS _{10.0}	0.010	9.2592	10.0000	-7.4
4	100PPBCNS _{100.0}	0.091	100.5680	100.0000	6.6
5	250PPBCNS _{250.0}	0.225	251.8372	250.0000	0.7
6	500PPBCNS _{500.0}	0.444	498.9938	500.0000	-0.2

06/26/2024
RM