


LB131441

7471B

INSTRUMENT ID: CV1

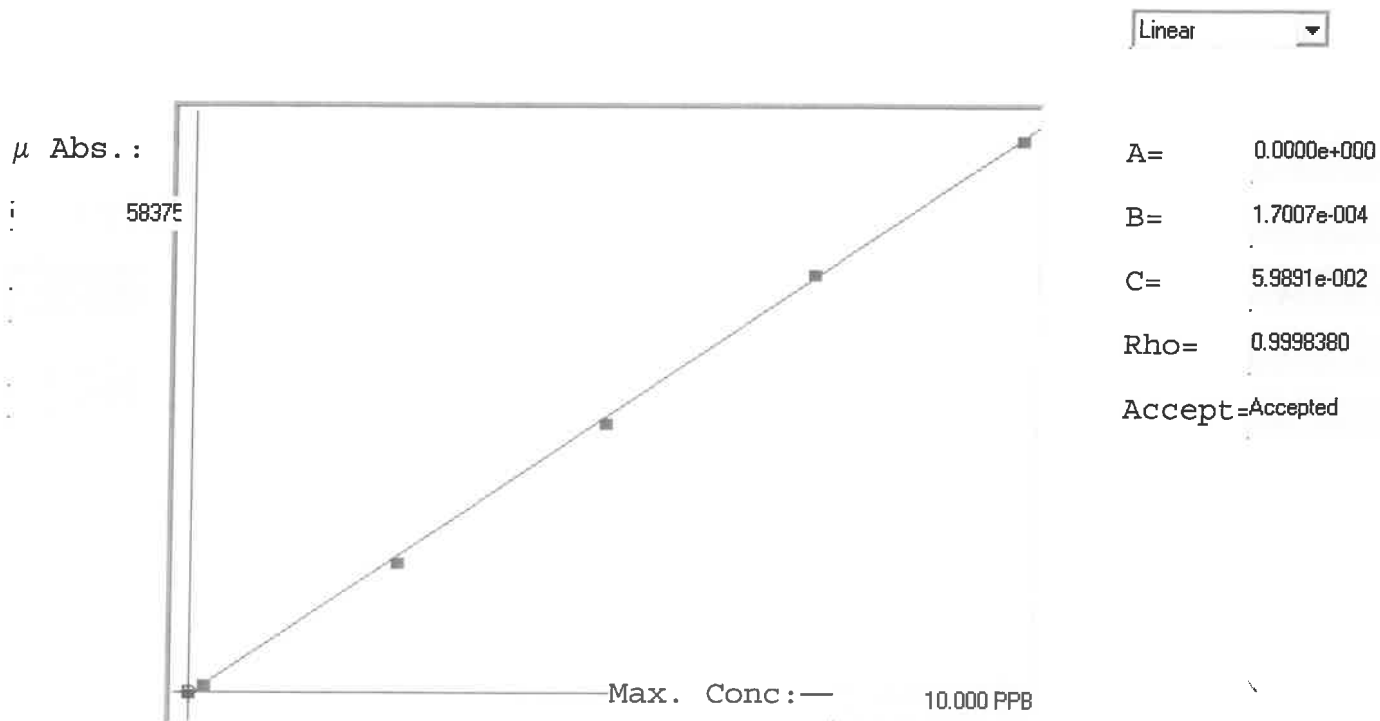

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.065	0.065	29	0.000	29					1
0.2	0.200	0.213	0.013	899	0.0 %	899					6
2.5	2.500	2.427	-0.073	13916	0.0 %	13916					3
5.0	5.000	4.913	-0.087	28538	0.0 %	28538					2
7.5	7.500	7.595	0.095	44307	0.0 %	44307					1
10.0	10.000	9.988	-0.012	58375	0.0 %	58375					0

LB131441 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 28 Jun 2024 12:33:08

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	20	29	-	0.0000	7471B	PPB	28 Jun 2024 12:39:05	S	Std
0.2 - 1	50.2	899	-	0.2000	7471B	PPB	28 Jun 2024 12:41:22	S	Std
2.5 - 1	52.5	13916	-	2.5000	7471B	PPB	28 Jun 2024 12:43:39	S	Std
5.0 - 1	55	28538	-	5.0000	7471B	PPB	28 Jun 2024 12:48:39	S	Std
7.5 - 1	57.5	44307	-	7.5000	7471B	PPB	28 Jun 2024 12:53:43	S	Std
10.0 - 1	510	58375	-	10.0000	7471B	PPB	28 Jun 2024 13:01:27	S	Std
ICV10 - 1	ICV10	25121	4.3321	-	7471B	PPB	28 Jun 2024 13:06:51	U	SMPL
ICB10 - 1	ICB10	-207	0.0247	-	7471B	PPB	28 Jun 2024 13:09:08	U	SMPL
CCV13 - 1	CCV13	28985	4.9893	-	7471B	PPB	28 Jun 2024 13:11:27	U	SMPL
CCB13 - 1	CCB13	-197	0.0264	-	7471B	PPB	28 Jun 2024 13:13:42	U	SMPL
CRA - 1	CRA	897	0.2124	-	7471B	PPB	28 Jun 2024 13:16:03	U	SMPL
HighStd - 1	HighStd	58305	9.9756	-	7471B	PPB	28 Jun 2024 13:18:18	U	SMPL
PB161813BL - 1	PBS	161	0.0873	-	7471B	PPB	28 Jun 2024 13:23:00	U	SMPL
PB161813BS - 1	LCSS	21430	3.7044	-	7471B	PPB	28 Jun 2024 13:25:16	U	SMPL
P3064-01 - 1	HD-02-062524	5863	1.0570	-	7471B	PPB	28 Jun 2024 13:27:32	U	SMPL
P3069-01 - 1	52924	693	0.1777	-	7471B	PPB	28 Jun 2024 13:29:51	U	SMPL
P3072-04 - 1	1419	226	0.0983	-	7471B	PPB	28 Jun 2024 13:32:10	U	SMPL
P3076-01 - 1	7-N-1	5777	1.0424	-	7471B	PPB	28 Jun 2024 13:34:27	U	SMPL
P3076-04 - 1	7-W-1	4680	0.8558	-	7471B	PPB	28 Jun 2024 13:36:43	U	SMPL
CCV14 - 1	CCV14	28043	4.8291	-	7471B	PPB	28 Jun 2024 13:39:01	U	SMPL
CCB14 - 1	CCB14	-229	0.0209	-	7471B	PPB	28 Jun 2024 13:41:18	U	SMPL
P3076-07 - 1	7-E-1	7220	1.2878	-	7471B	PPB	28 Jun 2024 13:43:37	U	SMPL
P3076-10 - 1	7-S-1	7401	1.3186	-	7471B	PPB	28 Jun 2024 13:45:53	U	SMPL
P3076-13 - 1	7-B-1	7324	1.3055	-	7471B	PPB	28 Jun 2024 13:48:10	U	SMPL
P3077-01 - 1	1-N-1	6344	1.1388	-	7471B	PPB	28 Jun 2024 13:50:28	U	SMPL
P3077-04 - 1	1-W-1	6590	1.1806	-	7471B	PPB	28 Jun 2024 13:52:46	U	SMPL
P3077-07 - 1	1-S-1	6430	1.1534	-	7471B	PPB	28 Jun 2024 13:55:04	U	SMPL
P3077-10 - 1	1-B-1	7351	1.3101	-	7471B	PPB	28 Jun 2024 14:02:26	U	SMPL
P3077-10DUP - 1	1-B-1DUP	7137	1.2737	-	7471B	PPB	28 Jun 2024 14:04:42	U	SMPL
P3077-10MS - 1	1-B-1MS	29711	5.1127	-	7471B	PPB	28 Jun 2024 14:07:01	U	SMPL
P3077-10MSD - 1	1-B-1MSD	30644	5.2714	-	7471B	PPB	28 Jun 2024 14:09:18	U	SMPL
CCV15 - 1	CCV15	28607	4.9250	-	7471B	PPB	28 Jun 2024 14:11:38	U	SMPL
CCB15 - 1	CCB15	-216	0.0232	-	7471B	PPB	28 Jun 2024 14:13:58	U	SMPL
P3077-10LX5 - 1		1433	0.3036	-	7471B	PPB	28 Jun 2024 14:16:18	U	SMPL
P3077-10A - 1		28360	4.8830	-	7471B	PPB	28 Jun 2024 14:18:33	U	SMPL
ChkStd - 1	ChkStd	38989	6.6906	-	7471B	PPB	28 Jun 2024 14:27:07	U	SMPL
CCV16 - 1	CCV16	30538	5.2534	-	7471B	PPB	28 Jun 2024 14:29:44	U	SMPL
CCB16 - 1	CCB16	-336	0.0027	-	7471B	PPB	28 Jun 2024 14:32:01	U	SMPL