


LB131472

7470A

INSTRUMENT ID: CV1

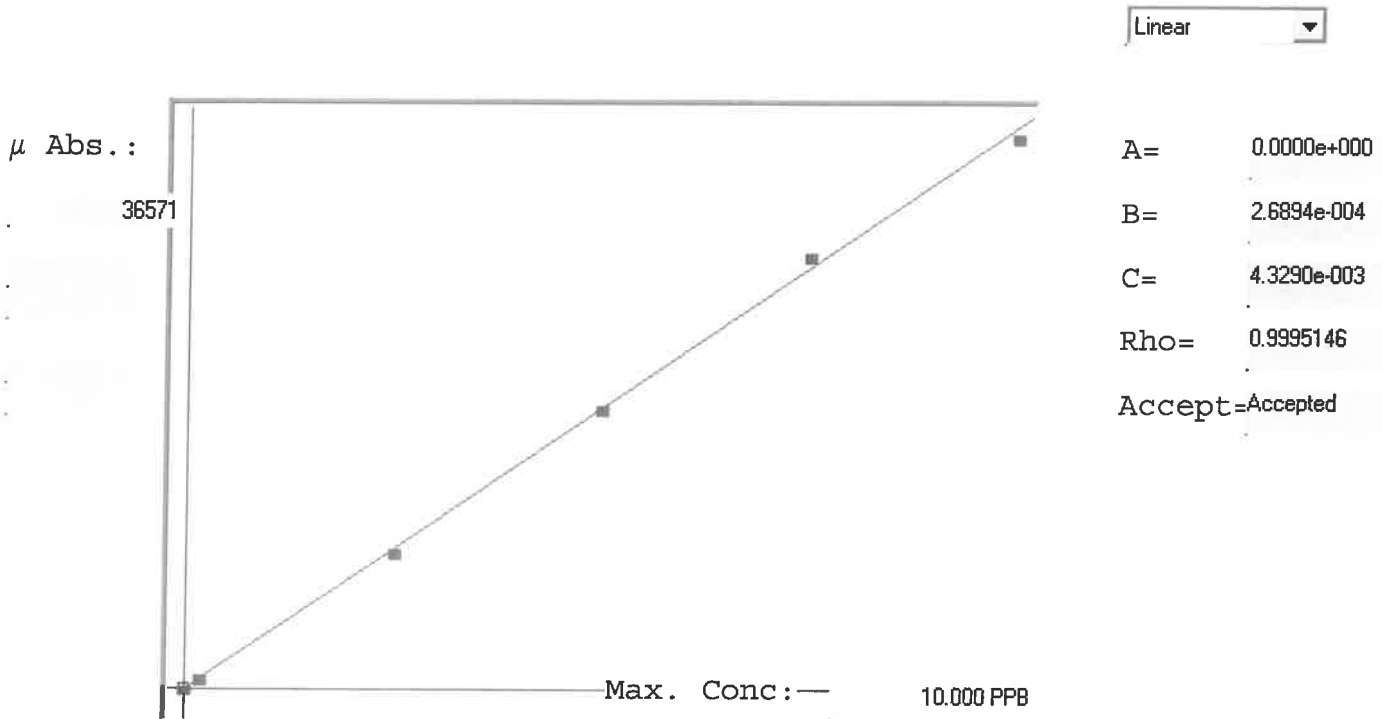

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	0/01
0.0	0.000	0.004	0.004	-1	0.000	-1	0				-6
0.2	0.200	0.189	-0.011	688	0.0 %	688					-2
2.5	2.500	2.448	-0.052	9088	0.0 %	9088					0
5.0	5.000	4.993	-0.007	18551	0.0 %	18551					3
7.5	7.500	7.725	0.225	28709	0.0 %	28709					2
10.0	10.000	9.840	-0.160	36571	0.0 %	36571					

LB131472 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 02 Jul 2024 12:51:58

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-1	-	0.0000	7470A	PPB	02 Jul 2024 13:28:14	S	Std
0.2 - 1	50-2	688	-	0.2000	7470A	PPB	02 Jul 2024 13:30:31	S	Std
2.5 - 1	52.5	9088	-	2.5000	7470A	PPB	02 Jul 2024 13:32:49	S	Std
5.0 - 1	55	18551	-	5.0000	7470A	PPB	02 Jul 2024 13:35:05	S	Std
7.5 - 1	57.5	28709	-	7.5000	7470A	PPB	02 Jul 2024 13:37:25	S	Std
10.0 - 1	510	36571	-	10.0000	7470A	PPB	02 Jul 2024 13:39:43	S	Std
ICV15 - 1	ICV15	13524	3.6414	-	7470A	PPB	02 Jul 2024 13:42:40	U	SMPL
ICB15 - 1	ICB15	-233	-0.0583	-	7470A	PPB	02 Jul 2024 13:44:55	U	SMPL
CCV29 - 1	CCV29	18785	0.5063	-	7470A	PPB	02 Jul 2024 13:47:12	U	SMPL
CCB29 - 1	CCB29	-263	-0.0664	-	7470A	PPB	02 Jul 2024 13:49:28	U	SMPL
CRA - 1	CRA	632	0.1743	-	7470A	PPB	02 Jul 2024 13:51:45	U	SMPL
HighStd - 1	HighStd	36238	9.7500	-	7470A	PPB	02 Jul 2024 13:54:00	U	SMPL
ChkStd - 1	ChkStd	26956	7.2538	-	7470A	PPB	02 Jul 2024 13:56:15	U	SMPL
PB161845BL - 1	PBW	-379	-0.0976	-	7470A	PPB	02 Jul 2024 13:58:34	U	SMPL
PB161845BS - 1	LCSW	13211	3.5572	-	7470A	PPB	02 Jul 2024 14:00:52	U	SMPL
P3106-01 - 1	S-1	-87	-0.0191	-	7470A	PPB	02 Jul 2024 14:03:08	U	SMPL
P3106-02 - 1	S-2	6	0.0059	-	7470A	PPB	02 Jul 2024 14:05:27	U	SMPL
P3106-03 - 1	S-3	42	0.0156	-	7470A	PPB	02 Jul 2024 14:07:43	U	SMPL
P3115-01 - 1	D3547	-1	0.0041	-	7470A	PPB	02 Jul 2024 14:10:00	U	SMPL
P3115-02 - 1	D3534	44	0.0162	-	7470A	PPB	02 Jul 2024 14:12:15	U	SMPL
CCV30 - 1	CCV30	18105	4.8734	-	7470A	PPB	02 Jul 2024 14:14:31	U	SMPL
CCB30 - 1	CCB30	-221	-0.0551	-	7470A	PPB	02 Jul 2024 14:16:47	U	SMPL
P3115-03 - 1	D3585	-29	-0.0035	-	7470A	PPB	02 Jul 2024 14:19:04	U	SMPL
P3115-06 - 1	D3526-27	-15	0.0003	-	7470A	PPB	02 Jul 2024 14:21:19	U	SMPL
P3115-07 - 1	D3588-89	-16	0.0000	-	7470A	PPB	02 Jul 2024 14:23:35	U	SMPL
P3116-01 - 1	D248	-9	0.0019	-	7470A	PPB	02 Jul 2024 14:25:51	U	SMPL
P3116-02 - 1	D249	101	0.0315	-	7470A	PPB	02 Jul 2024 14:28:07	U	SMPL
P3134-02 - 1	VNJ-238	-30	-0.0037	-	7470A	PPB	02 Jul 2024 14:30:23	U	SMPL
P3135-06 - 1	OK-628-COMP-01	-15	0.0003	-	7470A	PPB	02 Jul 2024 14:32:39	U	SMPL
P3135-12 - 1	OK-628-COMP-02	-10	0.0016	-	7470A	PPB	02 Jul 2024 14:34:57	U	SMPL
P3135-12DUP - 1	OK-628-COMP-02DUP	3	0.0051	-	7470A	PPB	02 Jul 2024 14:37:15	U	SMPL
P3135-12MS - 1	OK-628-COMP-02MS	14393	3.8751	-	7470A	PPB	02 Jul 2024 14:39:30	U	SMPL
CCV31 - 1	CCV31	18482	4.9748	-	7470A	PPB	02 Jul 2024 14:41:46	U	SMPL
CCB31 - 1	CCB31	-267	-0.0675	-	7470A	PPB	02 Jul 2024 14:44:04	U	SMPL
P3135-12MSD - 1	OK-628-COMP-02MSD	14689	3.9547	-	7470A	PPB	02 Jul 2024 14:46:21	U	SMPL
PB161848BL - 1	PBW	-209	-0.0519	-	7470A	PPB	02 Jul 2024 14:48:37	U	SMPL
PB161848BS - 1	LCSW	16776	4.5160	-	7470A	PPB	02 Jul 2024 14:50:54	U	SMPL
P3115-04 - 1	D3566	-181	-0.0443	-	7470A	PPB	02 Jul 2024 14:53:10	U	SMPL
P3115-05 - 1	D3591-93	-46	-0.0080	-	7470A	PPB	02 Jul 2024 14:55:27	U	SMPL
P3115-08 - 1	D3586-88-90	-29	-0.0035	-	7470A	PPB	02 Jul 2024 14:57:44	U	SMPL
P3115-09 - 1	T3565	-16	0.0000	-	7470A	PPB	02 Jul 2024 15:00:00	U	SMPL
P3115-10 - 1	T3558	-27	-0.0029	-	7470A	PPB	02 Jul 2024 15:02:17	U	SMPL
P3115-11 - 1	T3531	4	0.0054	-	7470A	PPB	02 Jul 2024 15:04:35	U	SMPL
P3116-03 - 1	D252	6	0.0059	-	7470A	PPB	02 Jul 2024 15:06:51	U	SMPL
CCV32 - 1	CCV32	18080	4.8667	-	7470A	PPB	02 Jul 2024 15:09:06	U	SMPL
CCB32 - 1	CCB32	-236	-0.0591	-	7470A	PPB	02 Jul 2024 15:11:22	U	SMPL
P3120-01 - 1	WC-2040627	-33	-0.0045	-	7470A	PPB	02 Jul 2024 15:13:40	U	SMPL
P3120-01DUP - 1	WC-2040627DUP	-3	0.0035	-	7470A	PPB	02 Jul 2024 15:15:56	U	SMPL
P3120-01MS - 1	WC-2040627MS	15386	4.1422	-	7470A	PPB	02 Jul 2024 15:18:11	U	SMPL
P3120-01MSD - 1	WC-2040627MSD	14703	3.9585	-	7470A	PPB	02 Jul 2024 15:20:27	U	SMPL
PB161885BL - 1	PBW	-188	-0.0462	-	7470A	PPB	02 Jul 2024 15:22:44	U	SMPL
PB161885BS - 1	LCSW	12680	3.4144	-	7470A	PPB	02 Jul 2024 15:25:03	U	SMPL
P3110-05 - 1	651	738	0.2028	-	7470A	PPB	02 Jul 2024 15:27:19	U	SMPL
P3110-05DUP - 1	651DUP	769	0.2111	-	7470A	PPB	02 Jul 2024 15:29:38	U	SMPL
P3110-05MS - 1	651MS	9793	2.6380	-	7470A	PPB	02 Jul 2024 15:31:55	U	SMPL
P3110-05MSD - 1	651MSD	9048	2.4377	-	7470A	PPB	02 Jul 2024 15:34:13	U	SMPL
CCV33 - 1	CCV33	17740	4.7753	-	7470A	PPB	02 Jul 2024 15:36:31	U	SMPL
CCB33 - 1	CCB33	-242	-0.0608	-	7470A	PPB	02 Jul 2024 15:38:49	U	SMPL
P3110-06 - 1	652	3298	0.8913	-	7470A	PPB	02 Jul 2024 15:41:07	U	SMPL
PB161814TB - 1	PB161814TB	-241	-0.0605	-	7470A	PPB	02 Jul 2024 15:43:22	U	SMPL
PB161821TB - 1	PB161821TB	-3	0.0035	-	7470A	PPB	02 Jul 2024 15:45:40	U	SMPL
P3135-12LX5 - 1		13	0.0078	-	7470A	PPB	02 Jul 2024 15:47:55	U	SMPL
P3135-12A - 1		13910	3.7452	-	7470A	PPB	02 Jul 2024 15:50:11	U	SMPL
P3120-01LX5 - 1		-103	-0.0234	-	7470A	PPB	02 Jul 2024 15:52:26	U	SMPL
P3120-01A - 1		14220	3.8286	-	7470A	PPB	02 Jul 2024 15:54:45	U	SMPL
P3110-05LX5 - 1		13	0.0078	-	7470A	PPB	02 Jul 2024 15:57:03	U	SMPL
P3110-05A - 1		13340	3.5919	-	7470A	PPB	02 Jul 2024 15:59:22	U	SMPL
CCV34 - 1	CCV34	17766	4.7822	-	7470A	PPB	02 Jul 2024 16:01:39	U	SMPL
CCB34 - 1	CCB34	-266	-0.0672	-	7470A	PPB	02 Jul 2024 16:03:57	U	SMPL