

LB 131533


7470A

INSTRUMENT ID: CY1

Linear

 μ Abs.:

34417

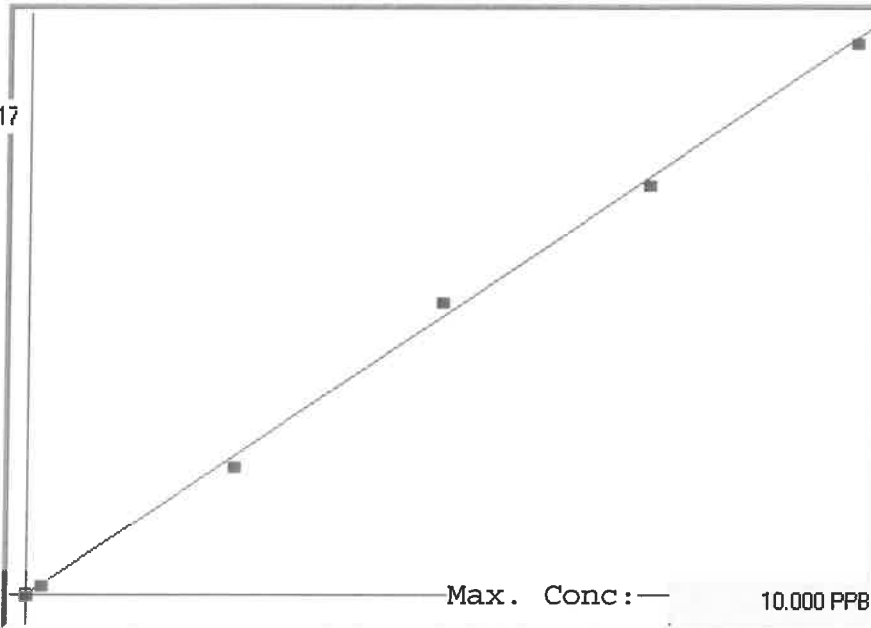

A= 0.0000e+000

B= 2.8878e-004

C= 1.7516e-002

Rho= 0.9991433

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.016	0.016	-5	0.000	-5	0				-
0.2	0.200	0.203	0.003	641	0.0 %	641					-2
2.5	2.500	2.324	-0.176	7987	0.0 %	7987					-7
5.0	5.000	5.309	0.309	18322	0.0 %	18322					6
7.5	7.500	7.392	-0.108	25538	0.0 %	25538					-1
10.0	10.000	9.956	-0.044	34417	0.0 %	34417					0

LB131533 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 08 Jul 2024 13:32:40

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-5	-	0.0000	7470A	PPB	08 Jul 2024 13:37:08	S	Std
0.2 - 1	50.2	641	-	0.2000	7470A	PPB	08 Jul 2024 13:39:25	S	Std
2.5 - 1	52.5	7987	-	2.5000	7470A	PPB	08 Jul 2024 13:41:42	S	Std
5.0 - 1	55	18322	-	5.0000	7470A	PPB	08 Jul 2024 13:44:00	S	Std
7.5 - 1	57.5	25538	-	7.5000	7470A	PPB	08 Jul 2024 13:46:17	S	Std
10.0 - 1	59	34417	-	10.0000	7470A	PPB	08 Jul 2024 13:53:47	S	Std
ICV20 - 1	ICV20	14264	4.1367	-	7470A	PPB	08 Jul 2024 14:01:57	U	SMPL
ICB20 - 1	ICB20	-262	-0.0581	-	7470A	PPB	08 Jul 2024 14:04:13	U	SMPL
CCV52 - 1	CCV52	18627	5.3966	-	7470A	PPB	08 Jul 2024 14:11:57	U	SMPL
CCB52 - 1	CCB52	-262	-0.0581	-	7470A	PPB	08 Jul 2024 14:14:11	U	SMPL
CRA - 1	CRA	596	0.1896	-	7470A	PPB	08 Jul 2024 14:16:29	U	SMPL
HighStd - 1	HighStd	34003	9.8369	-	7470A	PPB	08 Jul 2024 14:18:44	U	SMPL
ChkStd - 1	ChkStd	21621	6.2612	-	7470A	PPB	08 Jul 2024 14:21:00	U	SMPL
PB161960BL - 1	PBW	-319	-0.0746	-	7470A	PPB	08 Jul 2024 14:23:18	U	SMPL
PB161960BS - 1	LCSW	15005	4.3506	-	7470A	PPB	08 Jul 2024 14:28:21	U	SMPL
P3152-09 - 1	44-W	25760	7.4565	-	7470A	PPB	08 Jul 2024 14:35:47	U	SMPL
P3152-09DUP - 1	44-WDUP	23700	6.8616	-	7470A	PPB	08 Jul 2024 14:38:04	U	SMPL
P3152-09MS - 1	44-WMS	42953	12.4214	-	7470A	PPB	08 Jul 2024 14:40:24	U	SMPL
P3152-09MSD - 1	44-WMSD	40946	11.8419	-	7470A	PPB	08 Jul 2024 14:42:44	U	SMPL
P3160-02 - 1	COMP	174	0.0678	-	7470A	PPB	08 Jul 2024 14:45:02	U	SMPL
CCV53 - 1	CCV53	16516	4.7870	-	7470A	PPB	08 Jul 2024 14:47:20	U	SMPL
CCB53 - 1	CCB53	-233	-0.0498	-	7470A	PPB	08 Jul 2024 14:49:36	U	SMPL
P3152-09LX5 - 1		5847	1.7060	-	7470A	PPB	08 Jul 2024 14:51:54	U	SMPL
P3152-09A - 1		40113	11.6013	-	7470A	PPB	08 Jul 2024 14:54:09	U	SMPL
P3152-09DLX2 - 1		13478	3.9097	-	7470A	PPB	08 Jul 2024 14:56:26	U	SMPL
P3152-09DUPDLX2 - 1		12179	3.5346	-	7470A	PPB	08 Jul 2024 14:58:46	U	SMPL
P3152-09MSDLX2 - 1		20648	5.9802	-	7470A	PPB	08 Jul 2024 15:01:03	U	SMPL
P3152-09MSDDLX2 - 1		21076	6.1038	-	7470A	PPB	08 Jul 2024 15:03:22	U	SMPL
P3152-09LDLX10 - 1		2213	0.6566	-	7470A	PPB	08 Jul 2024 15:05:41	U	SMPL
P3152-09ADLX2 - 1		17366	5.0325	-	7470A	PPB	08 Jul 2024 15:10:39	U	SMPL
CCV54 - 1	CCV54	17599	5.0997	-	7470A	PPB	08 Jul 2024 15:12:56	U	SMPL
CCB54 - 1	CCB54	-187	-0.0365	-	7470A	PPB	08 Jul 2024 15:15:13	U	SMPL