


LB131569

7470A

INSTRUMENT ID: CV1

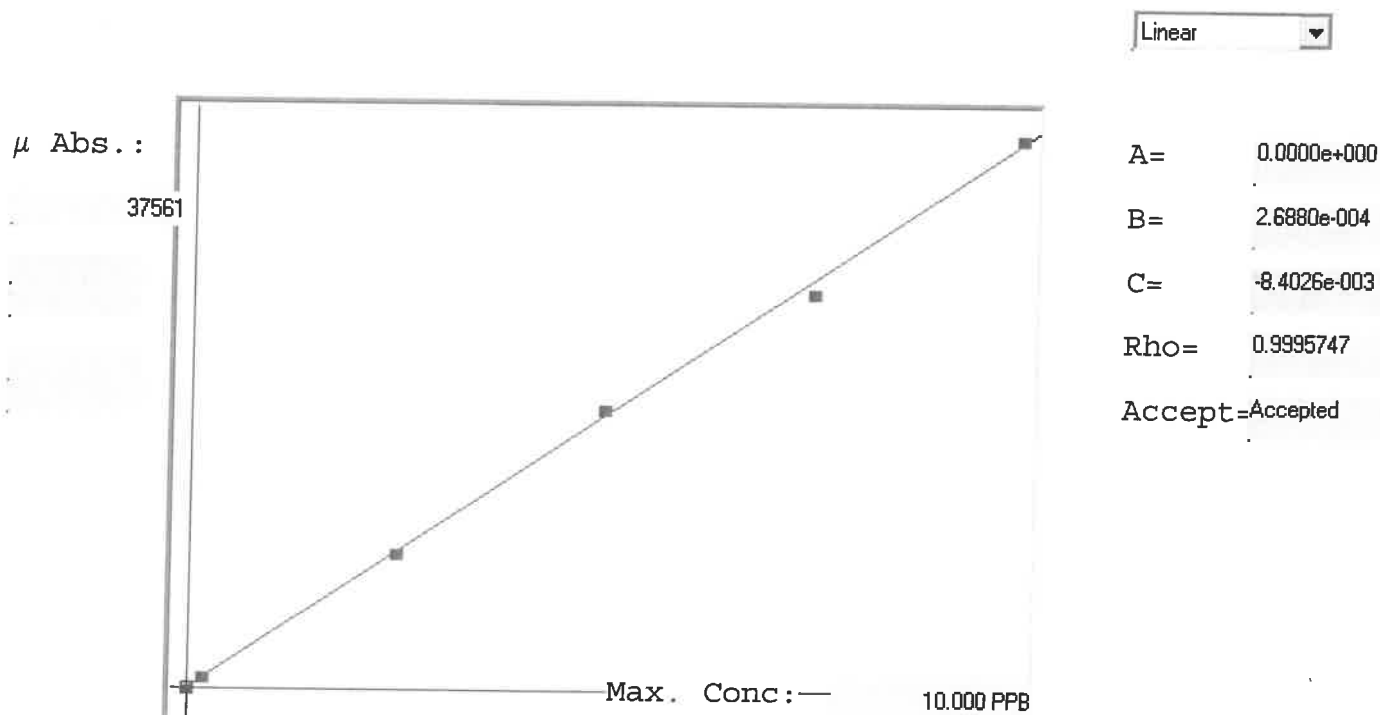

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%h
0.0	0.000	0.009	0.009	66	0.000	66	0				-
0.2	0.200	0.201	0.001	780	0.0 %	780					1
2.5	2.500	2.475	-0.025	9239	0.0 %	9239					-1
5.0	5.000	5.134	0.134	19131	0.0 %	19131					3
7.5	7.500	7.292	-0.208	27161	0.0 %	27161					-3
10.0	10.000	10.088	0.088	37561	0.0 %	37561					1

LB131569 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 11 Jul 2024 09:43:00

Sample ID	Extended ID	μ Abs.	Conc.	Strnd Conc	Method	Units	Date	Type	Type
0.0 - 1	50	66	-	0.0000	7470A	PPB	11 Jul 2024 10:01:46	S	Std
0.2 - 1	50.2	780	-	0.2000	7470A	PPB	11 Jul 2024 10:04:03	S	Std
2.5 - 1	52.5	9239	-	2.5000	7470A	PPB	11 Jul 2024 10:06:20	S	Std
5.0 - 1	55	19131	-	5.0000	7470A	PPB	11 Jul 2024 10:08:37	S	Std
7.5 - 1	57.5	27161	-	7.5000	7470A	PPB	11 Jul 2024 10:13:49	S	Std
10.0 - 1	59.6	37561	-	10.0000	7470A	PPB	11 Jul 2024 10:16:05	S	Std
ICV24 - 1	ICV24	14321	3.8411	-	7470A	PPB	11 Jul 2024 10:34:20	U	SMPL
ICB24 - 1	ICB24	-176	-0.0557	-	7470A	PPB	11 Jul 2024 10:36:36	U	SMPL
CCV63 - 1	CCV63	19200	5.1525	-	7470A	PPB	11 Jul 2024 10:38:53	U	SMPL
CCB63 - 1	CCB63	-163	-0.0522	-	7470A	PPB	11 Jul 2024 10:41:08	U	SMPL
CRA - 1	CRA	693	0.1779	-	7470A	PPB	11 Jul 2024 10:46:20	U	SMPL
HighStd - 1	HighStd	36380	9.7705	-	7470A	PPB	11 Jul 2024 10:48:35	U	SMPL
ChkStd - 1	ChkStd	25629	6.8806	-	7470A	PPB	11 Jul 2024 10:50:50	U	SMPL
PB161997BL - 1	PBW	-271	-0.0812	-	7470A	PPB	11 Jul 2024 10:53:09	U	SMPL
PB161997BS - 1	LCSW	15402	4.1316	-	7470A	PPB	11 Jul 2024 10:55:27	U	SMPL
P3183-02 - 1	N28660	-56	-0.0235	-	7470A	PPB	11 Jul 2024 10:57:44	U	SMPL
P3183-06 - 1	VNJ-226	-31	-0.0167	-	7470A	PPB	11 Jul 2024 11:00:03	U	SMPL
P3183-08 - 1	VNJ-229	40	0.0023	-	7470A	PPB	11 Jul 2024 11:02:20	U	SMPL
P3184-03 - 1	COMP(00187-00189-00186)	95	0.0171	-	7470A	PPB	11 Jul 2024 11:04:37	U	SMPL
P3184-06 - 1	MOO-23-00199	93	0.0166	-	7470A	PPB	11 Jul 2024 11:06:53	U	SMPL
CCV64 - 1	CCV64	18881	5.0668	-	7470A	PPB	11 Jul 2024 11:09:08	U	SMPL
CCB64 - 1	CCB64	-216	-0.0665	-	7470A	PPB	11 Jul 2024 11:11:23	U	SMPL
P3186-04 - 1	WC-4	38	0.0018	-	7470A	PPB	11 Jul 2024 11:13:41	U	SMPL
P3187-04 - 1	WC-1	80	0.0131	-	7470A	PPB	11 Jul 2024 11:15:56	U	SMPL
P3187-08 - 1	WC-2	96	0.0174	-	7470A	PPB	11 Jul 2024 11:18:11	U	SMPL
P3187-12 - 1	WC-3	62	0.0083	-	7470A	PPB	11 Jul 2024 11:20:27	U	SMPL
P3187-12DUP - 1	WC-3DUP	-14	-0.0122	-	7470A	PPB	11 Jul 2024 11:22:43	U	SMPL
P3187-12MS - 1	WC-3MS	13694	3.6725	-	7470A	PPB	11 Jul 2024 11:24:59	U	SMPL
P3187-12MSD - 1	WC-3MSD	13958	3.7435	-	7470A	PPB	11 Jul 2024 11:30:04	U	SMPL
PB162006BL - 1	PBW	-199	-0.0619	-	7470A	PPB	11 Jul 2024 11:32:21	U	SMPL
PB162006BS - 1	LCSW	14811	3.9728	-	7470A	PPB	11 Jul 2024 11:37:24	U	SMPL
P3170-06 - 1	WATER-DRUMS	971	0.2526	-	7470A	PPB	11 Jul 2024 11:39:40	U	SMPL
CCV65 - 1	CCV65	18919	5.0770	-	7470A	PPB	11 Jul 2024 11:41:57	U	SMPL
CCB65 - 1	CCB65	-221	-0.0678	-	7470A	PPB	11 Jul 2024 11:44:12	U	SMPL
P3170-06DUP - 1	WATER-DRUMSDUP	1159	0.3031	-	7470A	PPB	11 Jul 2024 11:46:30	U	SMPL
P3170-06MS - 1	WATER-DRUMSMS	13995	3.7534	-	7470A	PPB	11 Jul 2024 11:54:27	U	SMPL
P3170-06MSD - 1	WATER-DRUMSMSD	14196	3.8075	-	7470A	PPB	11 Jul 2024 11:56:43	U	SMPL
PB161973TB - 1	PB161973TB	-289	-0.0861	-	7470A	PPB	11 Jul 2024 11:59:01	U	SMPL
P3187-12LX5 - 1		-20	-0.0138	-	7470A	PPB	11 Jul 2024 12:01:19	U	SMPL
P3187-12A - 1		17516	4.6999	-	7470A	PPB	11 Jul 2024 12:03:36	U	SMPL
P3170-06LX5 - 1		-21	-0.0140	-	7470A	PPB	11 Jul 2024 12:05:52	U	SMPL
P3170-06A - 1		14023	3.7610	-	7470A	PPB	11 Jul 2024 12:08:12	U	SMPL
CCV66 - 1	CCV66	18622	4.9972	-	7470A	PPB	11 Jul 2024 12:10:29	U	SMPL
CCB66 - 1	CCB66	-4	-0.0095	-	7470A	PPB	11 Jul 2024 12:15:21	U	SMPL