

LB131655


7470A

INSTRUMENT ID: CY2

Linear

 μ Abs.:

40726

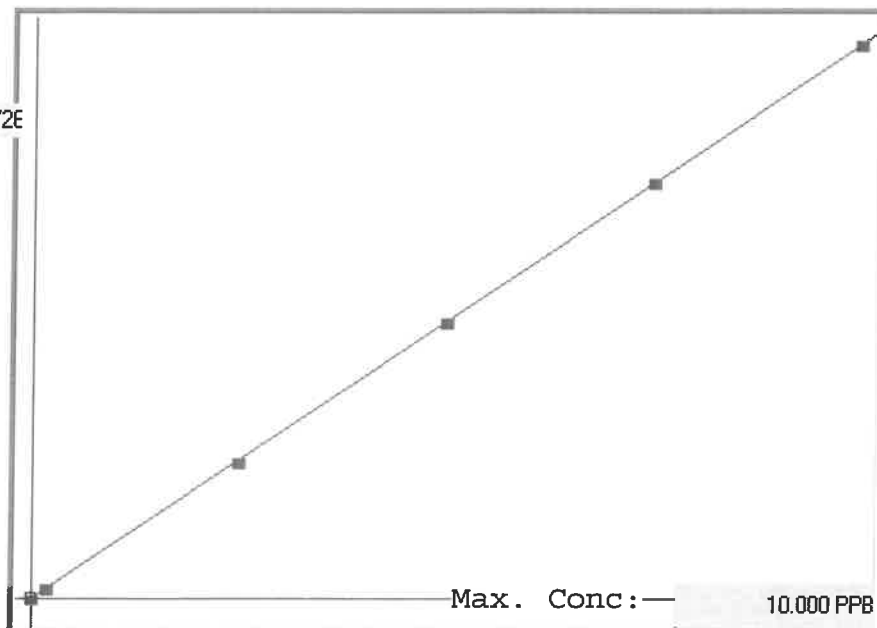

A= 0.0000e+000

B= 2.4514e-004

C= 9.9348e-003

Rho= 0.9999918

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	
0.0	0.000	0.019	0.019	37	0.000	37	0				0/00
0.2	0.200	0.192	-0.008	743	0.0 %	743					14
2.5	2.500	2.475	-0.025	10054	0.0 %	10054					15
5.0	5.000	5.011	0.011	20401	0.0 %	20401					00
7.5	7.500	7.510	0.010	30596	0.0 %	30596					00
10.0	10.000	9.993	-0.007	40726	0.0 %	40726					00

LB131655 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 18 Jul 2024 09:02:01

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	80	37	-	0.0000	7470A	PPB	18 Jul 2024 09:36:26	S	Std
0.2 - 1	50.2	743	-	0.2000	7470A	PPB	18 Jul 2024 09:38:43	S	Std
2.5 - 1	52.5	10054	-	2.5000	7470A	PPB	18 Jul 2024 09:41:01	S	Std
5.0 - 1	55	20401	-	5.0000	7470A	PPB	18 Jul 2024 09:43:18	S	Std
7.5 - 1	57.5	30596	-	7.5000	7470A	PPB	18 Jul 2024 09:45:36	S	Std
10.0 - 1	510	40726	-	10.0000	7470A	PPB	18 Jul 2024 09:53:40	S	Std
ICV34 - 1	ICV34	17261	4.2412	-	7470A	PPB	18 Jul 2024 09:59:24	U	SMPL
ICB34 - 1	ICB34	-209	-0.0413	-	7470A	PPB	18 Jul 2024 10:01:39	U	SMPL
CCV01 - 1	CCV01	21640	5.3147	-	7470A	PPB	18 Jul 2024 10:12:19	U	SMPL
CCB01 - 1	CCB01	-250	-0.0513	-	7470A	PPB	18 Jul 2024 10:14:33	U	SMPL
CRA - 1	CRA	680	0.1766	-	7470A	PPB	18 Jul 2024 10:16:51	U	SMPL
HighStd - 1	HighStd	40625	9.9686	-	7470A	PPB	18 Jul 2024 10:19:06	U	SMPL
ChkStd - 1	ChkStd	29354	7.2057	-	7470A	PPB	18 Jul 2024 10:24:07	U	SMPL
PB162117BL - 1	PBW	-347	-0.0751	-	7470A	PPB	18 Jul 2024 10:26:22	U	SMPL
PB162117BS - 1	LCSW	17149	4.2138	-	7470A	PPB	18 Jul 2024 10:28:41	U	SMPL
P3246-02 - 1	WC-CTW2-BL-01	-261	-0.0540	-	7470A	PPB	18 Jul 2024 10:30:57	U	SMPL
P3246-02DUP - 1	WC-CTW2-BL-01DUP	-10	0.0075	-	7470A	PPB	18 Jul 2024 10:33:16	U	SMPL
P3246-02MS - 1	WC-CTW2-BL-01MS	17204	4.2273	-	7470A	PPB	18 Jul 2024 10:35:33	U	SMPL
P3246-02MSD - 1	WC-CTW2-BL-01MSD	15382	3.7806	-	7470A	PPB	18 Jul 2024 10:37:49	U	SMPL
P3246-07 - 1	WC-CTW2-BL-02	-268	-0.0558	-	7470A	PPB	18 Jul 2024 10:40:07	U	SMPL
CCV02 - 1	CCV02	19442	4.7759	-	7470A	PPB	18 Jul 2024 10:42:24	U	SMPL
CCB02 - 1	CCB02	-223	-0.0447	-	7470A	PPB	18 Jul 2024 10:44:40	U	SMPL
P3246-12 - 1	WC-CTW2-BL-03	-19	0.0053	-	7470A	PPB	18 Jul 2024 10:47:03	U	SMPL
P3246-17 - 1	WC-CTW2-BL-04	23	0.0156	-	7470A	PPB	18 Jul 2024 10:49:26	U	SMPL
P3246-22 - 1	WC-CTW2-BL-05	-9	0.0077	-	7470A	PPB	18 Jul 2024 10:51:45	U	SMPL
P3246-27 - 1	WC-CTW2-BL-06	-8	0.0080	-	7470A	PPB	18 Jul 2024 10:54:00	U	SMPL
P3253-05 - 1	COMP-1	6	0.0114	-	7470A	PPB	18 Jul 2024 10:56:16	U	SMPL
P3253-06 - 1	COMP-2	28	0.0168	-	7470A	PPB	18 Jul 2024 10:58:33	U	SMPL
P3253-07 - 1	ELZ-24-00058	0	0.0099	-	7470A	PPB	18 Jul 2024 11:00:49	U	SMPL
P3254-01 - 1	72-11938	0	0.0099	-	7470A	PPB	18 Jul 2024 11:03:07	U	SMPL
P3254-03 - 1	SOM-24-00069	5	0.0112	-	7470A	PPB	18 Jul 2024 11:05:24	U	SMPL
P3254-04 - 1	COMP-1	0	0.0099	-	7470A	PPB	18 Jul 2024 11:07:40	U	SMPL
CCV03 - 1	CCV03	20048	4.9244	-	7470A	PPB	18 Jul 2024 11:12:41	U	SMPL
CCB03 - 1	CCB03	-250	-0.0513	-	7470A	PPB	18 Jul 2024 11:14:56	U	SMPL
P3254-05 - 1	COMP-2	-37	0.0009	-	7470A	PPB	18 Jul 2024 11:17:14	U	SMPL
P3266-04 - 1	SP-1-COMP	55	0.0234	-	7470A	PPB	18 Jul 2024 11:19:30	U	SMPL
P3266-08 - 1	SP-2-COMP	32	0.0178	-	7470A	PPB	18 Jul 2024 11:21:46	U	SMPL
PB162118BL - 1	PBW	-16	0.0060	-	7470A	PPB	18 Jul 2024 11:24:01	U	SMPL
PB162118BS - 1	LCSW	15913	3.9108	-	7470A	PPB	18 Jul 2024 11:27:14	U	SMPL
P3257-02 - 1	WC-W-03-202407	-190	-0.0366	-	7470A	PPB	18 Jul 2024 11:29:30	U	SMPL
P3257-02DUP - 1	WC-W-03-202407DUP	25	0.0161	-	7470A	PPB	18 Jul 2024 11:31:48	U	SMPL
P3257-02MS - 1	WC-W-03-202407MS	13343	3.2808	-	7470A	PPB	18 Jul 2024 11:34:06	U	SMPL
P3257-02MSD - 1	WC-W-03-202407MSD	15936	3.9164	-	7470A	PPB	18 Jul 2024 11:36:23	U	SMPL
P3258-02 - 1	WC-W-02-202407	-213	-0.0423	-	7470A	PPB	18 Jul 2024 11:38:41	U	SMPL
CCV04 - 1	CCV04	19712	4.8421	-	7470A	PPB	18 Jul 2024 11:40:58	U	SMPL
CCB04 - 1	CCB04	-213	-0.0423	-	7470A	PPB	18 Jul 2024 11:43:14	U	SMPL
PB162075TB - 1	PB162075TB	-47	-0.0016	-	7470A	PPB	18 Jul 2024 11:45:31	U	SMPL
PB162092TB - 1	PB162092TB	9	0.0121	-	7470A	PPB	18 Jul 2024 11:47:47	U	SMPL
PB162093TB - 1	PB162093TB	-13	0.0067	-	7470A	PPB	18 Jul 2024 11:50:03	U	SMPL
P3246-02LX5 - 1		3	0.0107	-	7470A	PPB	18 Jul 2024 11:52:18	U	SMPL
P3246-02A - 1		16179	3.9760	-	7470A	PPB	18 Jul 2024 11:54:34	U	SMPL
P3257-02LX5 - 1		-108	-0.0165	-	7470A	PPB	18 Jul 2024 11:56:50	U	SMPL
P3257-02A - 1		16285	4.0020	-	7470A	PPB	18 Jul 2024 11:59:09	U	SMPL
CCV05 - 1	CCV05	19636	4.8234	-	7470A	PPB	18 Jul 2024 12:01:26	U	SMPL
CCB05 - 1	CCB05	-198	-0.0386	-	7470A	PPB	18 Jul 2024 12:03:44	U	SMPL