


LB131741

SFAM01.1

INSTRUMENT ID: CV1

Linear

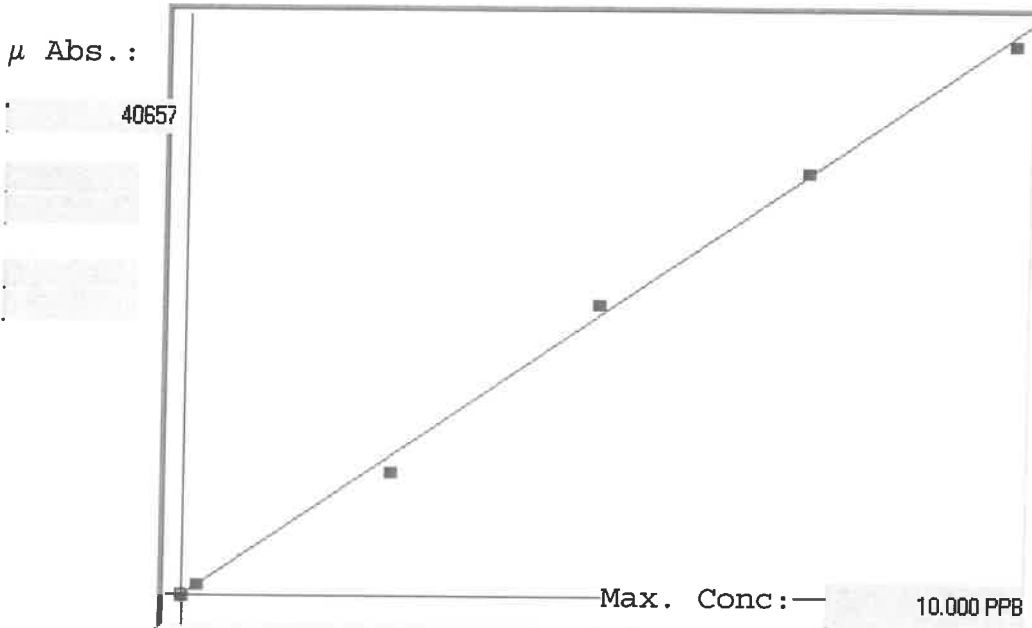

A= 0.0000e+000

B= 2.4229e-004 slope

C= 1.1591e-002 $r = \text{mlwcept}$

Rho= 0.9990582

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	o/b)
0.00	0.000	0.030	0.030	77	0.000	77					
0.05	0.050					442	0				
0.20	0.200	0.232	0.032	908	0.0 %	908					
2.50	2.500	2.246	-0.254	9222	0.0 %	9222					
5.00	5.000	5.249	0.249	21616	0.0 %	21616					
7.50	7.500	7.581	0.081	31239	0.0 %	31239					
10.0	10.000	9.863	-0.137	40657	0.0 %	40657					

o/b)
= 16
- 10
5
- 1

LB131741

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	77	-		0 SFAM01.1	PPB	7/25/2024 14:47	Std
	0.2 S01	908	-		0.2 SFAM01.1	PPB	7/25/2024 14:49	Std
	2.5 S02	9222	-		2.5 SFAM01.1	PPB	7/25/2024 14:51	Std
	5 S03	21616	-		5 SFAM01.1	PPB	7/25/2024 14:59	Std
	7.5 S04	31239	-		7.5 SFAM01.1	PPB	7/25/2024 15:01	Std
	10 S05	40657	-		10 SFAM01.1	PPB	7/25/2024 15:08	Std
ICV045	ICV045	16634	4.0419 -		SFAM01.1	PPB	7/25/2024 15:11	SMPL
ICB045	ICB045	-110	-0.0151 -		SFAM01.1	PPB	7/25/2024 15:13	SMPL
CCV041	CCV041	21272	5.1657 -		SFAM01.1	PPB	7/25/2024 15:15	SMPL
CCB041	CCB041	-126	-0.0189 -		SFAM01.1	PPB	7/25/2024 15:17	SMPL
PB162278BL	PBW278	47	0.023 -		SFAM01.1	PPB	7/25/2024 15:20	SMPL
P3349-01	E08H7	56	0.0252 -		SFAM01.1	PPB	7/25/2024 15:22	SMPL
P3349-02	E08H7D	49	0.0235 -		SFAM01.1	PPB	7/25/2024 15:24	SMPL
P3349-03	E08H7S	4358	1.0675 -		SFAM01.1	PPB	7/25/2024 15:26	SMPL
P3349-04	E08H9	75	0.0298 -		SFAM01.1	PPB	7/25/2024 15:29	SMPL
P3351-01	E08H4	54	0.0247 -		SFAM01.1	PPB	7/25/2024 15:31	SMPL
P3350-01	E08H7	30	0.0189 -		SFAM01.1	PPB	7/25/2024 15:33	SMPL
P3350-02	E08H7D	61	0.0264 -		SFAM01.1	PPB	7/25/2024 15:35	SMPL
P3350-03	E08H7S	4955	1.2122 -		SFAM01.1	PPB	7/25/2024 15:38	SMPL
P3350-04	E08H9	131	0.0433 -		SFAM01.1	PPB	7/25/2024 15:40	SMPL
CCV042	CCV042	20925	5.0816 -		SFAM01.1	PPB	7/25/2024 15:42	SMPL
CCB042	CCB042	-120	-0.0175 -		SFAM01.1	PPB	7/25/2024 15:44	SMPL