

|      |          |
|------|----------|
| N    | 11       |
| Mean | 64.756   |
| SD   | 100.9445 |
| CV%  | 155.88   |

Aquakem v. 7.2AQ1

Results from time period:

Thu Jul 25 14:09:19 2024

Thu Jul 25 14:47:27 2024

| Sample Id         | Sam/Ctr/c/ | Test short  | Test type | Result   | Result unit | Result date and time |
|-------------------|------------|-------------|-----------|----------|-------------|----------------------|
| S0.0              | A          | CNEPA-NE\ P |           | 0.254    | µg/l        | 7/25/2024 14:09:19   |
| S5.0              | A          | CNEPA-NE\ P |           | 4.7668   | µg/l        | 7/25/2024 14:09:20   |
| S10.0             | A          | CNEPA-NE\ P |           | 9.6088   | µg/l        | 7/25/2024 14:09:21   |
| S100.0            | A          | CNEPA-NE\ P |           | 98.0528  | µg/l        | 7/25/2024 14:09:22   |
| S250.0            | A          | CNEPA-NE\ P |           | 253.8361 | µg/l        | 7/25/2024 14:09:23   |
| S500.0            | A          | CNEPA-NE\ P |           | 498.4815 | µg/l        | 7/25/2024 14:09:24   |
| ICV001 ICV001     | S          | CNEPA-NE\ P |           | 95.0332  | µg/l        | 7/25/2024 14:42:08   |
| ICB001 ICB001     | S          | CNEPA-NE\ P |           | 0.7272   | µg/l        | 7/25/2024 14:42:10   |
| CCV001 CCV001     | S          | CNEPA-NE\ P |           | 249.9625 | µg/l        | 7/25/2024 14:42:12   |
| CCB001 CCB001     | S          | CNEPA-NE\ P |           | 0.5647   | µg/l        | 7/25/2024 14:42:14   |
| PB162264BL PBW264 | S          | CNEPA-NE\ P |           | 0.8009   | µg/l        | 7/25/2024 14:42:15   |
| P3349-01 E08H7    | S          | CNEPA-NE\ P |           | 2.0694   | µg/l        | 7/25/2024 14:42:17   |
| P3349-02 E08H7D   | S          | CNEPA-NE\ P |           | 2.0314   | µg/l        | 7/25/2024 14:47:22   |
| P3349-03 E08H7S   | S          | CNEPA-NE\ P |           | 103.0447 | µg/l        | 7/25/2024 14:47:23   |
| P3349-04 E08H9    | S          | CNEPA-NE\ P |           | 0.3032   | µg/l        | 7/25/2024 14:47:24   |
| CCV002 CCV002     | S          | CNEPA-NE\ P |           | 256.6755 | µg/l        | 7/25/2024 14:47:26   |
| CCB002 CCB002     | S          | CNEPA-NE\ P |           | 1.1007   | µg/l        | 7/25/2024 14:47:27   |

CHEMTECH CONSULTING GROUP INC  
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : NF Instrument ID : Konelab

7/25/2024 14:10


Test CNEPA-NEW

Accepted 7/25/2024 14:10

Factor slope ~~1161~~ 0.000861  
Bias ~~0.001~~  
y-intercept

Coeff. of det. 0.999893

Errors

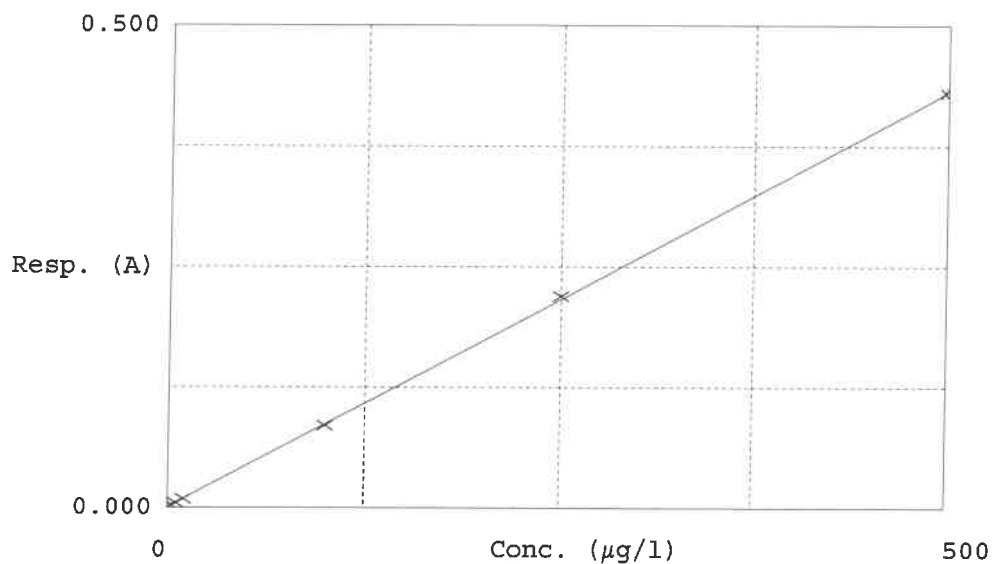

|   | Calibrator     | Response | Calc. con. | Conc.    | Re<br>Errors |
|---|----------------|----------|------------|----------|--------------|
| 1 | 0.0PPBCN 0.0   | 0.001    | 0.2540     | 0.0000   | -            |
| 2 | 5.0PPBCN 5.0   | 0.005    | 4.7668     | 5.0000   | -4.7         |
| 3 | 10PPBCN 10.0   | 0.009    | 9.6088     | 10.0000  | -3.9         |
| 4 | 100PPBCN 100.0 | 0.085    | 98.0528    | 100.0000 | -1.9         |
| 5 | 250PPBCN 250.0 | 0.219    | 253.8361   | 250.0000 | 1.5          |
| 6 | 500PPBCN 500.0 | 0.430    | 498.4815   | 500.0000 | -0.3         |

NF  
07.25.2024