


LB131748

7470A

INSTRUMENT ID: CV1

Linear

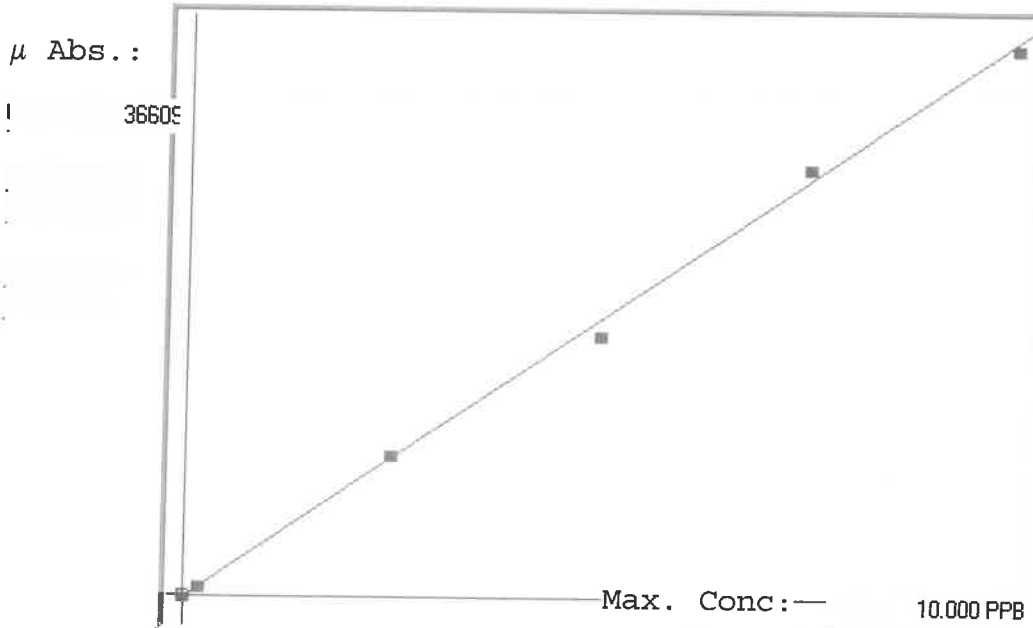

A= 0.0000e+000

B= 2.6983e-004

C= 2.9029e-002

Rho= 0.9990136

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	1.1)
0.0	0.000	0.019	0.019	-39	0.000	-39	0				1
0.2	0.200	0.207	0.007	661	0.0 %	661					3
2.5	2.500	2.586	0.086	9478	0.0 %	9478					3
5.0	5.000	4.722	-0.278	17391	0.0 %	17391					6
7.5	7.500	7.759	0.259	28648	0.0 %	28648					3
10.0	10.000	9.907	-0.093	36609	0.0 %	36609					1

LB131748 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 26 Jul 2024 13:38:28

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	80	-39	-	0.0000	7470A	PPB	26 Jul 2024 13:44:49	S	Std
0.2 - 1	51.2	661	-	0.2000	7470A	PPB	26 Jul 2024 13:47:05	S	Std
2.5 - 1	52.5	9478	-	2.5000	7470A	PPB	26 Jul 2024 13:49:22	S	Std
5.0 - 1	55	17391	-	5.0000	7470A	PPB	26 Jul 2024 13:51:39	S	Std
7.5 - 1	57.5	28648	-	7.5000	7470A	PPB	26 Jul 2024 13:53:57	S	Std
10.0 - 1	510	36609	-	10.0000	7470A	PPB	26 Jul 2024 13:59:24	S	Std
ICV46 - 1	ICV46	14602	3.9690	-	7470A	PPB	26 Jul 2024 14:02:11	U	SMPL
ICB46 - 1	ICB46	-170	-0.0168	-	7470A	PPB	26 Jul 2024 14:04:26	U	SMPL
CCV43 - 1	CCV43	19000	5.1557	-	7470A	PPB	26 Jul 2024 14:09:35	U	SMPL
CCB43 - 1	CCB43	-244	-0.0368	-	7470A	PPB	26 Jul 2024 14:11:51	U	SMPL
CRA - 1	CRA	689	0.2149	-	7470A	PPB	26 Jul 2024 14:14:08	U	SMPL
HighStd - 1	HighStd	36204	9.7978	-	7470A	PPB	26 Jul 2024 14:16:23	U	SMPL
ChkStd - 1	ChkStd	26206	7.1001	-	7470A	PPB	26 Jul 2024 14:18:38	U	SMPL
PB162301BL - 1	PBW	-318	-0.0568	-	7470A	PPB	26 Jul 2024 14:20:58	U	SMPL
PB162301BS - 1	LCSW	14035	3.8160	-	7470A	PPB	26 Jul 2024 14:23:17	U	SMPL
P3366-01 - 1	PRE	-176	-0.0185	-	7470A	PPB	26 Jul 2024 14:25:32	U	SMPL
P3366-02 - 1	POST	229	0.0908	-	7470A	PPB	26 Jul 2024 14:27:51	U	SMPL
CCV44 - 1	CCV44	18394	4.9922	-	7470A	PPB	26 Jul 2024 14:30:08	U	SMPL
CCB44 - 1	CCB44	-236	-0.0346	-	7470A	PPB	26 Jul 2024 14:32:25	U	SMPL