


LS131862

7470A INSTRUMENT ID: CV2

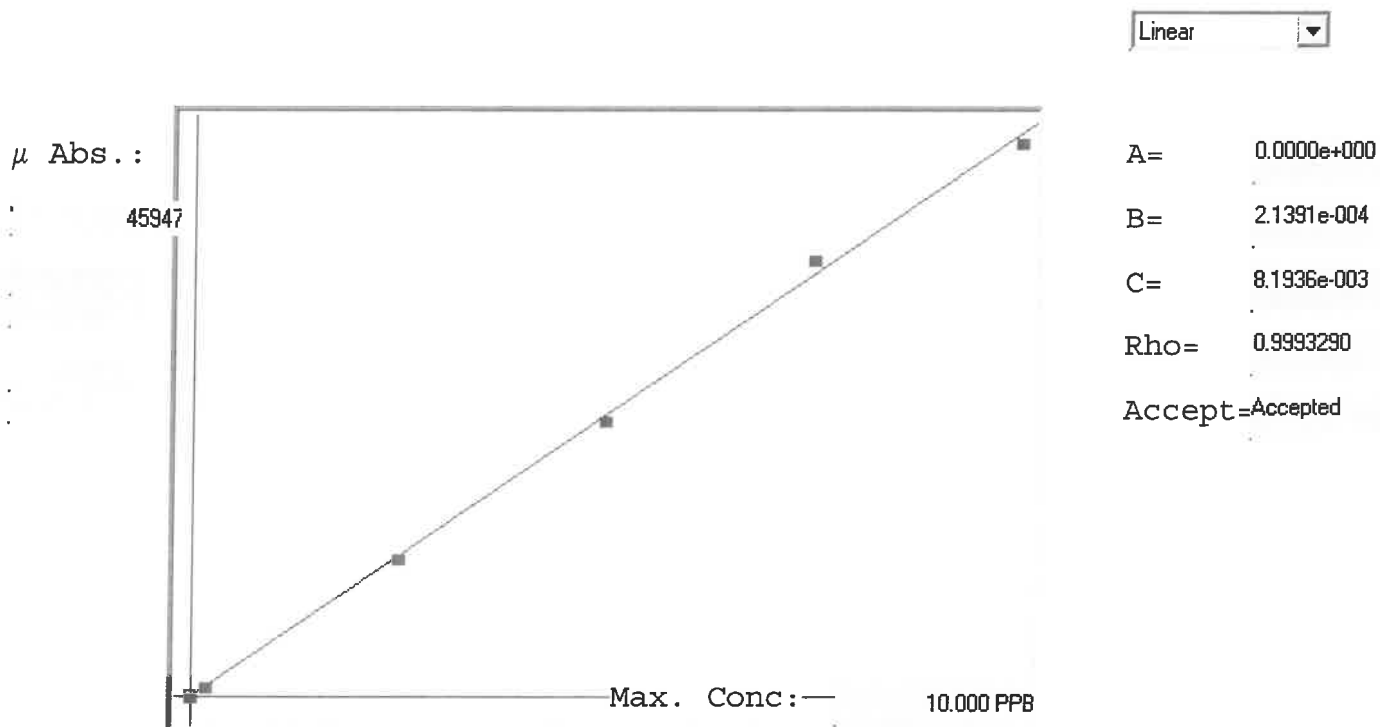

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.014	0.014	25	0.000	25	0				1
0.2	0.200	0.196	-0.004	878	0.0 %	878					2
2.5	2.500	2.470	-0.030	11507	0.0 %	11507					1
5.0	5.000	4.912	-0.088	22926	0.0 %	22926					2
7.5	7.500	7.772	0.272	36296	0.0 %	36296					4
10.0	10.000	9.837	-0.163	45947	0.0 %	45947					2

LB131862 INSTRUMENT ID; CV1

Method: 7470A

Operator: Admin

Date of Analysis: 05 Aug 2024 12:02:57

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	25	-	0.0000	7470A	PPB	05 Aug 2024 12:11:24	S	Std
0.2 - 1	50.2	878	-	0.2000	7470A	PPB	05 Aug 2024 12:13:41	S	Std
2.5 - 1	52.5	11507	-	2.5000	7470A	PPB	05 Aug 2024 12:15:58	S	Std
5.0 - 1	55	22926	-	5.0000	7470A	PPB	05 Aug 2024 12:18:14	S	Std
7.5 - 1	57.5	36296	-	7.5000	7470A	PPB	05 Aug 2024 12:20:31	S	Std
10.0 - 1	510	45947	-	10.0000	7470A	PPB	05 Aug 2024 12:22:48	S	Std
ICV59 - 1	ICV59	19033	4.0795	-	7470A	PPB	05 Aug 2024 12:25:33	U	SMPL
ICB59 - 1	ICB59	-88	-0.0106	-	7470A	PPB	05 Aug 2024 12:27:48	U	SMPL
CCV90 - 1	CCV90	22893	4.9051	-	7470A	PPB	05 Aug 2024 12:30:03	U	SMPL
CCB90 - 1	CCB90	-114	-0.0162	-	7470A	PPB	05 Aug 2024 12:32:18	U	SMPL
CRA - 1	CRA	911	0.2031	-	7470A	PPB	05 Aug 2024 12:34:34	U	SMPL
HighStd - 1	HighStd	44705	9.5709	-	7470A	PPB	05 Aug 2024 12:36:49	U	SMPL
ChkStd - 1	ChkStd	32515	6.9633	-	7470A	PPB	05 Aug 2024 12:39:04	U	SMPL
PB162491BL - 1	PB162491BL	-247	-0.0446	-	7470A	PPB	05 Aug 2024 12:41:22	U	SMPL
PB162491BS - 1	PB162491BS	17804	3.8166	-	7470A	PPB	05 Aug 2024 12:43:40	U	SMPL
P3419-01 - 1	286118	-125	-0.0185	-	7470A	PPB	05 Aug 2024 12:45:56	U	SMPL
P3419-01DUP - 1	286118DUP	4	0.0090	-	7470A	PPB	05 Aug 2024 12:48:14	U	SMPL
P3419-01MS - 1	286118MS	19064	4.0861	-	7470A	PPB	05 Aug 2024 12:50:30	U	SMPL
P3419-01MSD - 1	286118MSD	18514	3.9684	-	7470A	PPB	05 Aug 2024 12:52:48	U	SMPL
CCV91 - 1	CCV91	22425	4.8050	-	7470A	PPB	05 Aug 2024 12:55:04	U	SMPL
CCB91 - 1	CCB91	-186	-0.0316	-	7470A	PPB	05 Aug 2024 12:57:21	U	SMPL
PB162456TB - 1	PB162456TB	-4	0.0073	-	7470A	PPB	05 Aug 2024 12:59:37	U	SMPL
P3419-01LX5 - 1		31	0.0148	-	7470A	PPB	05 Aug 2024 13:01:53	U	SMPL
P3419-01A - 1		18448	3.9543	-	7470A	PPB	05 Aug 2024 13:04:08	U	SMPL
CCV92 - 1	CCV92	22186	4.7539	-	7470A	PPB	05 Aug 2024 13:06:23	U	SMPL
CCB92 - 1	CCB92	-12	0.0056	-	7470A	PPB	05 Aug 2024 13:08:41	U	SMPL