


LB131867

7471B

INSTRUMENT ID: CV1

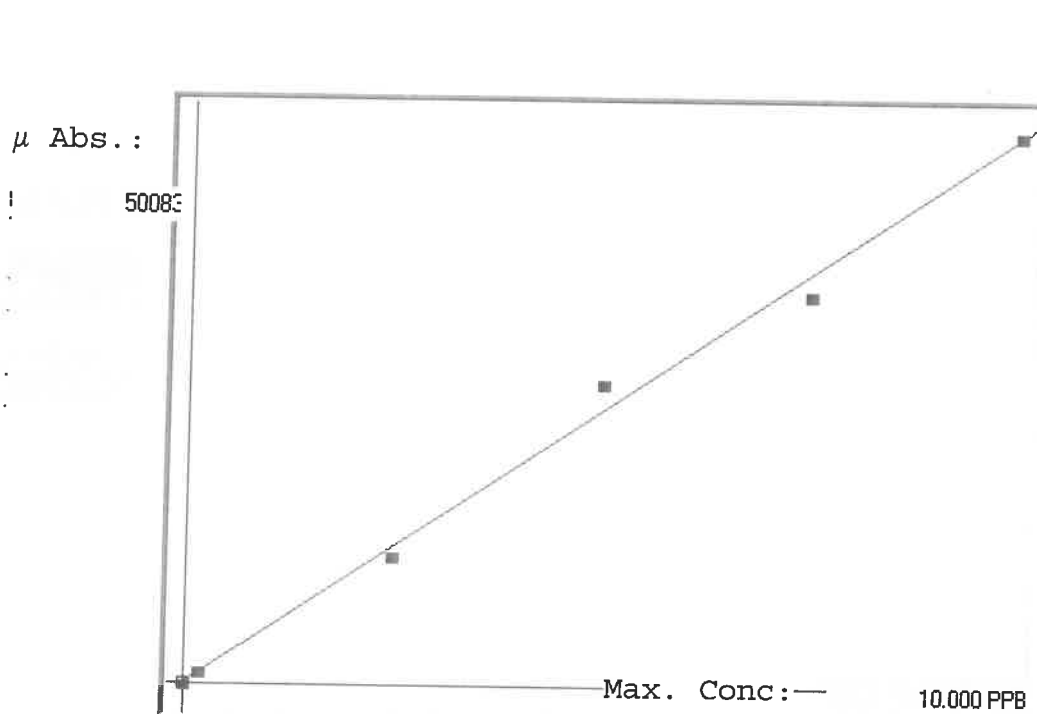

Linear

A= 0.0000e+000

B= 2.0059e-004

C= -1.2352e-002

Rho= 0.9975234

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	6/11
0.0	0.000	0.013	0.013	125	0.000	125					1
0.2	0.200	0.203	0.003	1074	0.0 %	1074					2
2.5	2.500	2.330	-0.170	11677	0.0 %	11677					7
5.0	5.000	5.488	0.488	27423	0.0 %	27423					10
7.5	7.500	7.132	-0.368	35617	0.0 %	35617					5
10.0	10.000	10.034	0.034	50083	0.0 %	50083					0

LB131867 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 05 Aug 2024 13:50:47

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	125	-	0.0000	7471B	PPB	05 Aug 2024 13:55:58	S	Std
0.2 - 1	50.2	1074	-	0.2000	7471B	PPB	05 Aug 2024 13:58:15	S	Std
2.5 - 1	52.5	11677	-	2.5000	7471B	PPB	05 Aug 2024 14:00:32	S	Std
5.0 - 1	55	27423	-	5.0000	7471B	PPB	05 Aug 2024 14:02:49	S	Std
7.5 - 1	57.5	35617	-	7.5000	7471B	PPB	05 Aug 2024 14:05:08	S	Std
10.0 - 1	510	50083	-	10.0000	7471B	PPB	05 Aug 2024 14:11:42	S	Std
ICV60 - 1	ICV60	18983	3.7954	-	7471B	PPB	05 Aug 2024 14:14:47	U	SMPL
ICB60 - 1	ICB60	-136	-0.0396	-	7471B	PPB	05 Aug 2024 14:17:02	U	SMPL
CCV93 - 1	CCV93	24937	4.9898	-	7471B	PPB	05 Aug 2024 14:19:20	U	SMPL
CCB93 - 1	CCB93	-160	-0.0444	-	7471B	PPB	05 Aug 2024 14:21:35	U	SMPL
CRA - 1	CRA	1009	0.1900	-	7471B	PPB	05 Aug 2024 14:23:53	U	SMPL
HighStd - 1	HighStd	49901	9.9973	-	7471B	PPB	05 Aug 2024 14:26:08	U	SMPL
ChkStd - 1	ChkStd	32339	6.4745	-	7471B	PPB	05 Aug 2024 14:28:24	U	SMPL
PB162498BL - 1	PBS	-222	-0.0569	-	7471B	PPB	05 Aug 2024 14:30:47	U	SMPL
PB162498BS - 1	LCSS	19712	3.9417	-	7471B	PPB	05 Aug 2024 14:33:09	U	SMPL
P3441-01 - 1	BU-02-08012024	2373	0.4636	-	7471B	PPB	05 Aug 2024 14:35:25	U	SMPL
P3441-01DUP - 1	BU-02-08012024DUP	2761	0.5415	-	7471B	PPB	05 Aug 2024 14:37:44	U	SMPL
P3441-01MS - 1	BU-02-08012024MS	22698	4.5406	-	7471B	PPB	05 Aug 2024 14:40:03	U	SMPL
P3441-01MSD - 1	BU-02-08012024MSD	23843	4.7703	-	7471B	PPB	05 Aug 2024 14:42:22	U	SMPL
P3442-01 - 1	CL-02-080124	9354	1.8640	-	7471B	PPB	05 Aug 2024 14:44:41	U	SMPL
CCV94 - 1	CCV94	25149	5.0323	-	7471B	PPB	05 Aug 2024 14:47:00	U	SMPL
CCB94 - 1	CCB94	-116	-0.0356	-	7471B	PPB	05 Aug 2024 14:49:17	U	SMPL
P3448-01 - 1	TP1	29907	5.9867	-	7471B	PPB	05 Aug 2024 14:51:35	U	SMPL
P3448-03 - 1	TP2	12596	2.5143	-	7471B	PPB	05 Aug 2024 14:53:49	U	SMPL
P3448-05 - 1	TP3	9795	1.9524	-	7471B	PPB	05 Aug 2024 14:56:09	U	SMPL
P3448-07 - 1	TP4	11541	2.3027	-	7471B	PPB	05 Aug 2024 14:58:27	U	SMPL
P3448-09 - 1	TP5	5007	0.9920	-	7471B	PPB	05 Aug 2024 15:00:44	U	SMPL
P3448-11 - 1	TP6	3567	0.7032	-	7471B	PPB	05 Aug 2024 15:03:03	U	SMPL
P3448-13 - 1	TP7	1730	0.3347	-	7471B	PPB	05 Aug 2024 15:05:20	U	SMPL
P3460-01 - 1	72-11929	3341	0.6578	-	7471B	PPB	05 Aug 2024 15:07:37	U	SMPL
P3461-01 - 1	CHRT-28607	4664	0.9232	-	7471B	PPB	05 Aug 2024 15:09:55	U	SMPL
P3462-03 - 1	JC-1-4-5	7561	1.5043	-	7471B	PPB	05 Aug 2024 15:12:11	U	SMPL
CCV95 - 1	CCV95	24864	4.9751	-	7471B	PPB	05 Aug 2024 15:14:28	U	SMPL
CCB95 - 1	CCB95	-89	-0.0302	-	7471B	PPB	05 Aug 2024 15:16:45	U	SMPL
P3462-07 - 1	JC-2	2509	0.4909	-	7471B	PPB	05 Aug 2024 15:19:03	U	SMPL
P3462-11 - 1	JC-3-6-7	671	0.1222	-	7471B	PPB	05 Aug 2024 15:21:18	U	SMPL
P3463-01 - 1	TR-04-082024	2491	0.4873	-	7471B	PPB	05 Aug 2024 15:23:34	U	SMPL
P3463-03 - 1	TR-05-082024	1051	0.1985	-	7471B	PPB	05 Aug 2024 15:25:50	U	SMPL
P3464-01 - 1	TOPSOIL	2124	0.4137	-	7471B	PPB	05 Aug 2024 15:28:06	U	SMPL
P3441-01LX5 - 1		365	0.0609	-	7471B	PPB	05 Aug 2024 15:30:22	U	SMPL
P3441-01A - 1		22811	4.5633	-	7471B	PPB	05 Aug 2024 15:32:38	U	SMPL
CCV96 - 1	CCV96	24992	5.0008	-	7471B	PPB	05 Aug 2024 15:34:55	U	SMPL
CCB96 - 1	CCB96	-65	-0.0254	-	7471B	PPB	05 Aug 2024 15:37:15	U	SMPL